



**CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS  
MAINTAINED IN THE REGULAR COURSE OF BUSINESS**

I, **Steven J. Carluccio**, Highway Safety Equipment Technical Supervisor, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NATL PATENT ANALYTICAL SYSTEM, DATAMASTER DMT breath test instrument, serial number 117106, performed on May 25, 2023 by Office of Public Safety employee Jonathan Mascolo, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance /calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink that reads "Steven J. Carluccio".

Digitally signed under ESRA  
by Steven J. Carluccio  
on 06/07/2023 10:32 AM

---

**Steven J. Carluccio**  
**Highway Safety Equipment Technical Supervisor**  
**Office of Public Safety**

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Glens Falls City Police Department

Manufacturer: NATL PATENT ANALYTICAL SYSTEM

Model: DATAMASTER DMT

Serial Number: 117106

Date: May 25, 2023

Reference Solution Lot Number : 23050

Reference Solution Standard : 0.10% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.101 %	34.00 degrees centigrade
2	0.100 %	34.00 degrees centigrade
3	0.101 %	34.00 degrees centigrade
4	0.101 %	34.00 degrees centigrade

Reference Solution Lot Number : 22210

Reference Solution Standard : 0.08% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.080 %	34.00 degrees centigrade
2	0.080 %	34.00 degrees centigrade
3	0.079 %	34.01 degrees centigrade
4	0.080 %	34.01 degrees centigrade

Reference Solution Lot Number : 22450

Reference Solution Standard : 0.18% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.179 %	34.02 degrees centigrade
2	0.179 %	34.02 degrees centigrade
3	0.179 %	34.02 degrees centigrade
4	0.179 %	34.02 degrees centigrade

I hereby certify that I have performed any necessary maintenance procedures and calibrated NATL PATENT ANALYTICAL SYSTEM breath test instrument model DATAMASTER DMT, serial number 117106, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.


I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.

Performed by:



Digitally signed under ESRA  
by Jonathan Mascolo  
on 05/25/2023 02:07 PM

Reviewed by:

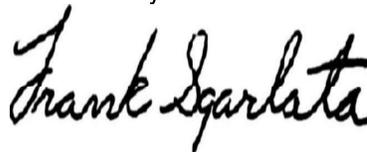

Digitally signed under ESRA  
by Frank Sgarlata  
on 05/25/2023 04:25 PM

**Jonathan Mascolo**  
Highway Safety Equipment Technician  
Breath Analysis Operator Permit #45339

**Frank Sgarlata**  
Breath Analysis Technical Supervisor

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

**Name of Submitting Agency: Glens Falls City Police Department**  
**Manufacturer: NATL PATENT ANALYTICAL SYSTEM**  
**Model: DATAMASTER DMT**  
**Serial Number: 117106**  
**Date: May 25, 2023**

- 1. General appearance and condition of this device -----: OK
  
- 2. Check controls and indicators -----: OK
  
- 3. Check breath flow system -----: OK
  
- 4. Check printer operation -----: OK
  
- 5. System cycles through all modes -----: OK



**6. Record any repairs made to this instrument and list services provided : INSPECTED INSTRUMENT, CHECKED SETUP VOLTAGES, PRINT AND REMOTE OPERATION. PERFORMED CALIBRATION/ADJUSTMENT PROCEDURE, RAN SUBJECT, TECHNICIAN AND DIAGNOSTIC TESTS, VERIFIED CALIBRATION.**

Performed by:

Handwritten signature of Jonathan Mascolo in black ink.

Digitally signed under ESRA  
by Jonathan Mascolo  
on 05/25/2023 02:07 PM

Reviewed by:

Handwritten signature of Frank Sgarlata in black ink.

Digitally signed under ESRA  
by Frank Sgarlata  
on 05/25/2023 04:25 PM

---

**Jonathan Mascolo**  
**Highway Safety Equipment Technician**  
**Breath Analysis Operator Permit #45339**

---

**Frank Sgarlata**  
**Breath Analysis Technical Supervisor**

TECHNICIAN TEST

-----  
GLENS FALLS CITY  
POLICE DEPT  
DATAMASTER dmt: 117106  
-----





Date: 05/25/2023

OPERATOR NAME:  
JONATHAN M MASCOLO  
Permit #: 45339  
Operator Agency/Dept: GLENS FALLS CITY PD  
Reference Standard #: 22210

Nominal = 0.080 g/210L

BLANK TEST	0.000	12:53
INTERNAL STANDARD	VERIFIED	12:54
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.080	12:54
BLANK TEST	0.000	12:55
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.080	12:55
BLANK TEST	0.000	12:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.079	12:56
BLANK TEST	0.000	12:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.080	12:58
BLANK TEST	0.000	12:58

Average = 0.0798  
Std Dev = 0.0005

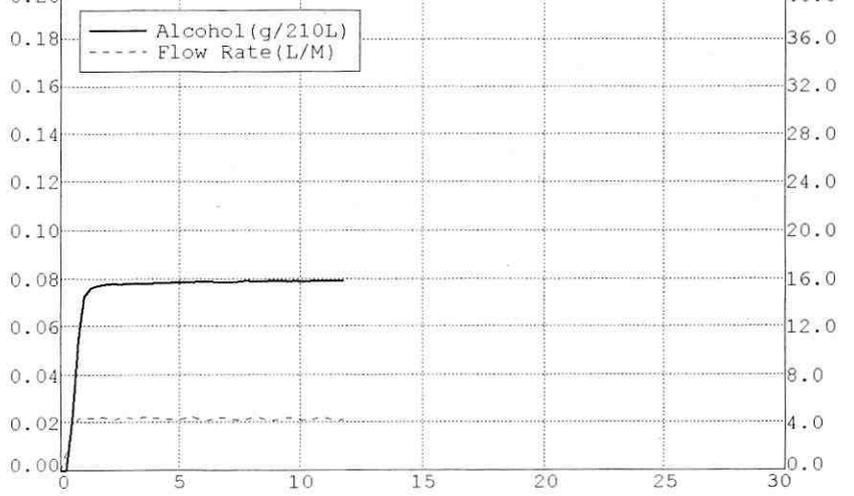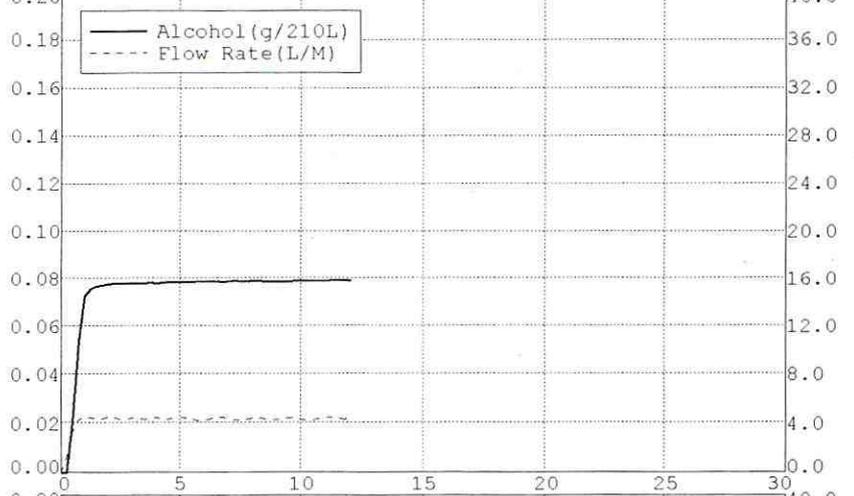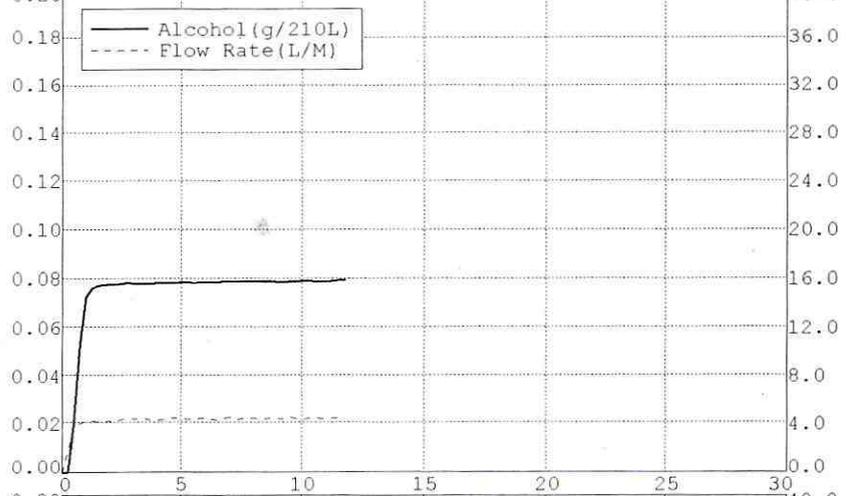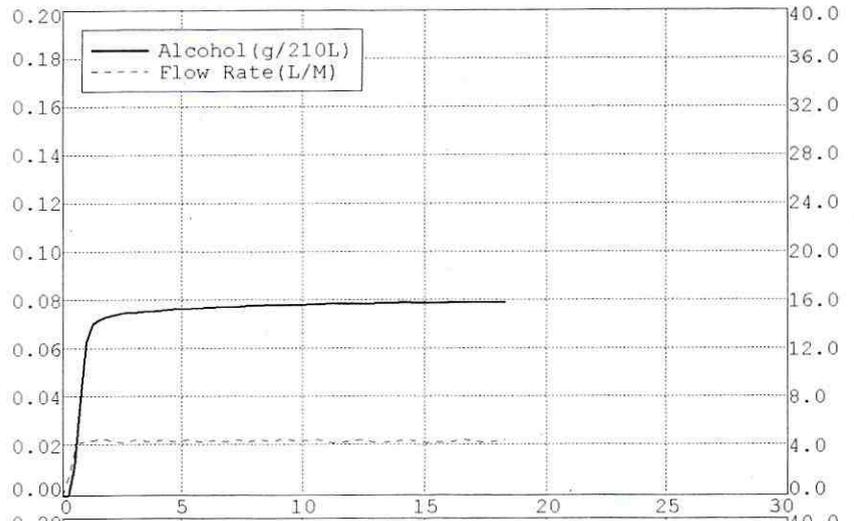

TECHNICIAN TEST

-----  
GLENS FALLS CITY  
POLICE DEPT  
DATAMASTER dmt: 117106  
-----





Date: 05/25/2023

OPERATOR NAME:  
JONATHAN M MASCOLO  
Permit #: 45339  
Operator Agency/Dept: GLENS FALLS CITY PD  
Reference Standard #: 23050

Nominal = 0.100 g/210L

BLANK TEST	0.000	13:01
INTERNAL STANDARD	VERIFIED	13:01
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.101	13:01
BLANK TEST	0.000	13:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.100	13:02
BLANK TEST	0.000	13:03
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.101	13:04
BLANK TEST	0.000	13:04
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.101	13:05
BLANK TEST	0.000	13:06

Average = 0.1008  
Std Dev = 0.0005

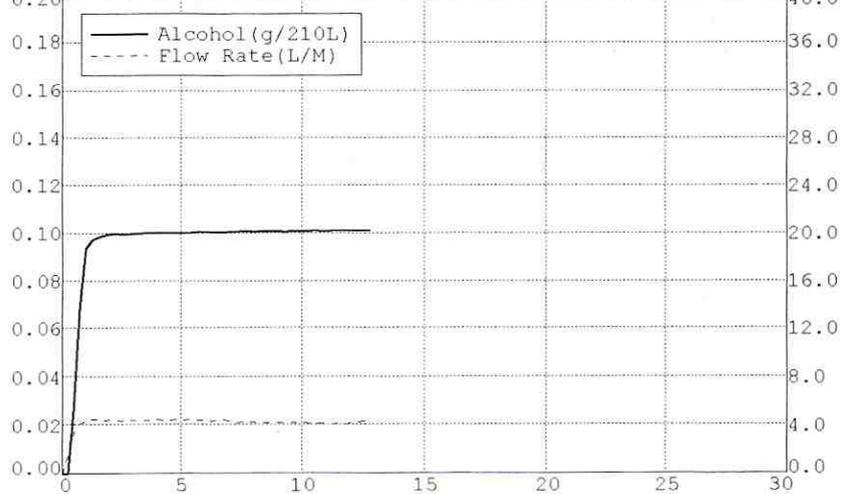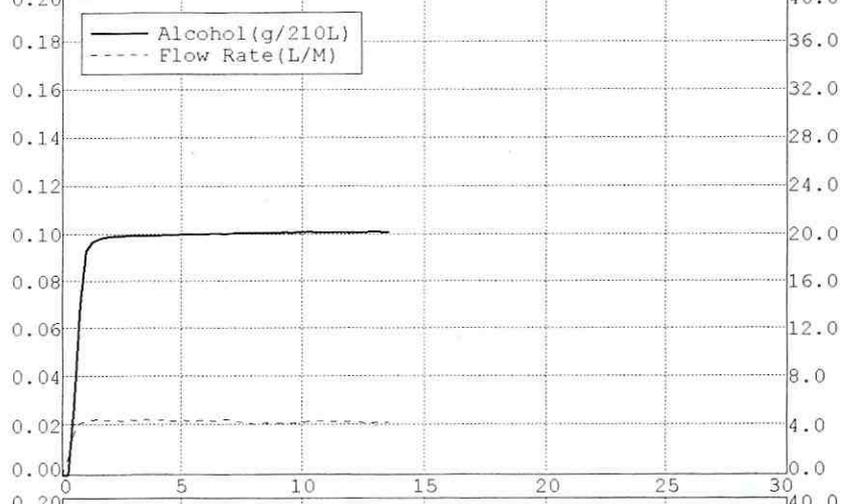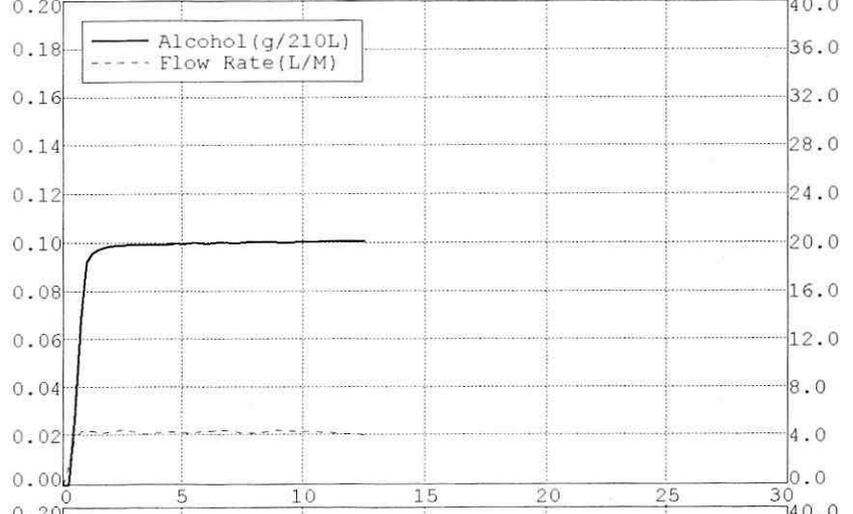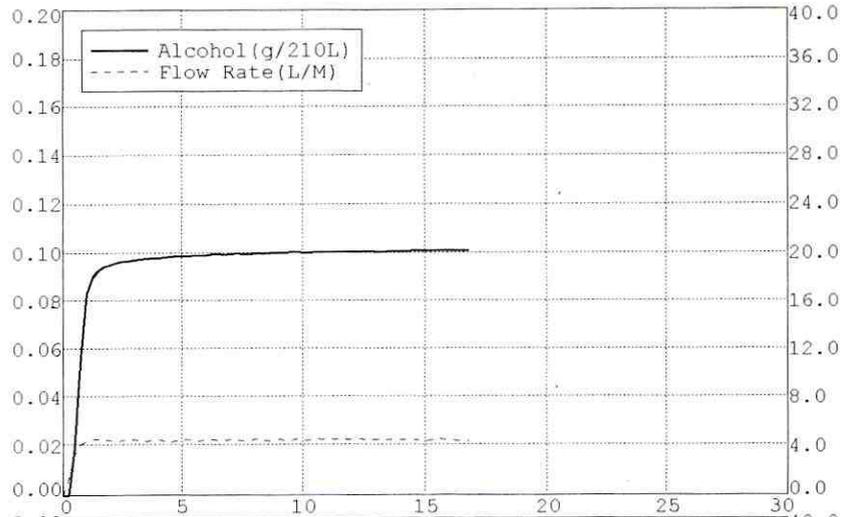

TECHNICIAN TEST

-----  
 GLENS FALLS CITY  
 POLICE DEPT  
 DATAMASTER dmt: 117106  
 -----





Date: 05/25/2023

OPERATOR NAME:  
 JONATHAN M MASCOLO  
 Permit #: 45339  
 Operator Agency/Dept: GLENS FALLS CITY PD  
 Reference Standard #: 22450

Nominal = 0.180 g/210L

BLANK TEST	0.000	13:08
INTERNAL STANDARD	VERIFIED	13:08
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.179	13:09
BLANK TEST	0.000	13:10
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.179	13:10
BLANK TEST	0.000	13:11
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.179	13:11
BLANK TEST	0.000	13:12
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.179	13:13
BLANK TEST	0.000	13:14

Average = 0.1790  
 Std Dev = 0.0000

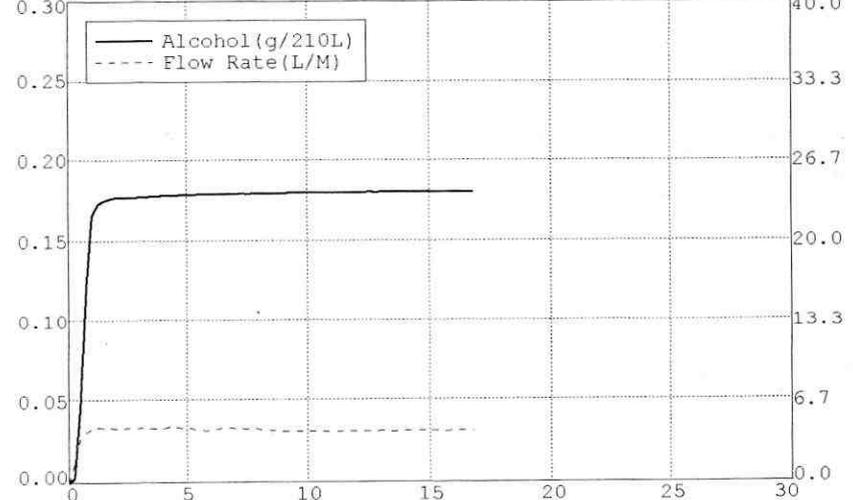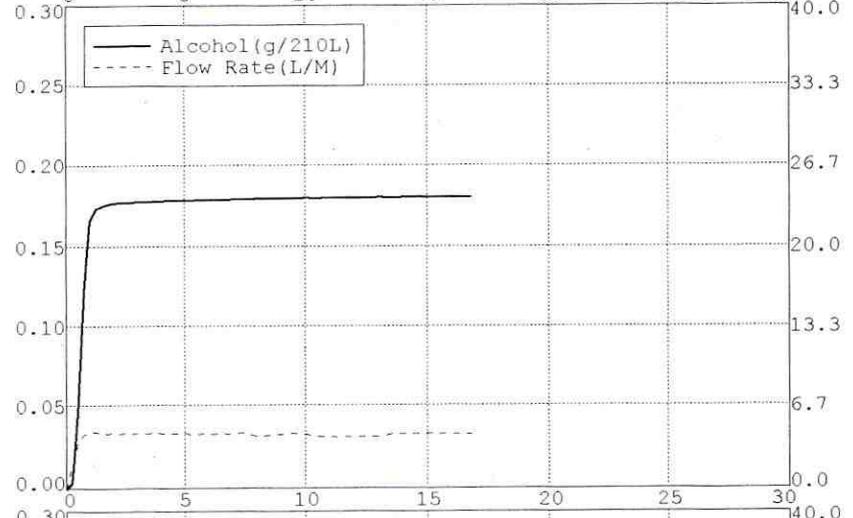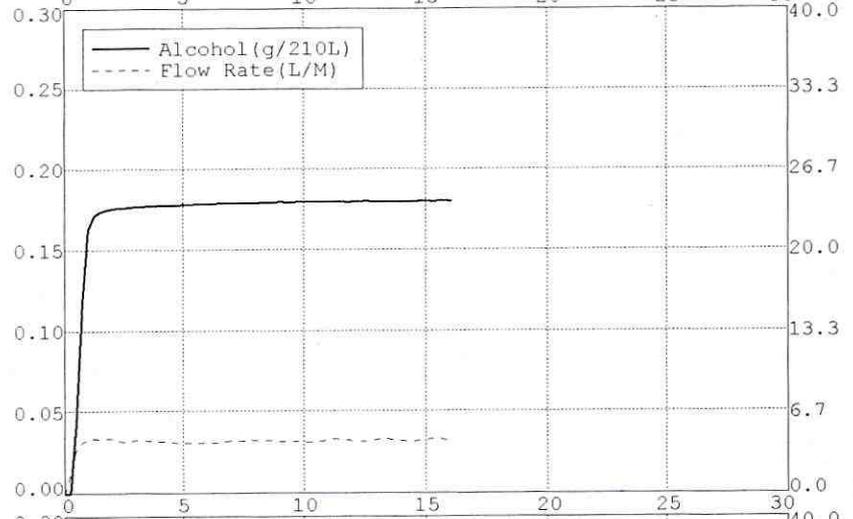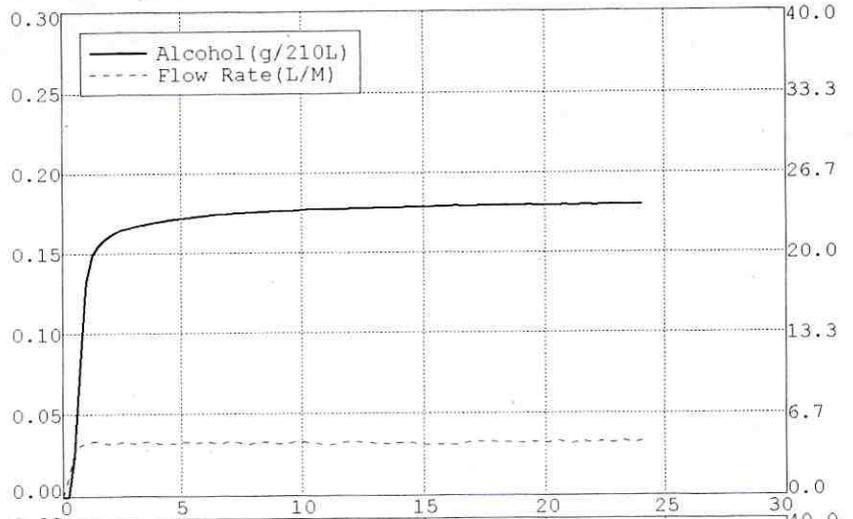

**SERVICE AUTHORIZATION FORM**  
**Highway Safety Technology Unit**  
**80 South Swan Street**  
**Albany, NY 12210**  
**Ph: 518-485-7636 / 518-402-0689**  
**Fax: 518-457-6869**

THIS FORM IS USED TO AUTHORIZE THE DIVISION OF CRIMINAL JUSTICE SERVICES TO PERFORM SERVICE ON THE INSTRUMENT IDENTIFIED. THIS AUTHORIZATION MUST ACCOMPANY EACH PIECE OF EQUIPMENT WHEN IT IS PRESENTED TO THE EQUIPMENT REPAIR CENTER FOR SERVICE. **PLEASE SIGN AND DATE FORM.**

**SECTION I – AGENCY INFORMATION**

Name of Agency Glens Falls Police Department		Today's Date 5/25/2023
Address 42 Ridge Street		City, State, ZIP Glens Falls, New York 12801
Contact Person LT. Ryan S. Pedone		Contact Telephone (518) 769-0596
Contact Email rpedone@glensfallspd.com		Best Way to Reach You During Appointment Period (518) 769-0596

**SECTION II – INSTRUMENT INFORMATION**

Instrument Manufacturer (Please Circle) NPAS DMT GUTH Applied Concepts (Stalker) Decatur (Genesis) Kustom (Eagle/Falcon) MPH Alco-Sensor Other:		
Model Number Datamaster DMT		Instrument Serial Number 117106
Antenna Serial Number (if applicable) Antenna 1 -- / Antenna 2 --		Type of maintenance (check appropriate) <input checked="" type="checkbox"/> Calibration Check <input type="checkbox"/> Repair
Brief Description of Malfunction Yearly Calibration		
List all parts, cables and/or accessories being submitted. Tuning forks must accompany all radar units (if applicable). (Please Circle)		
DMT/SIM: DMT 117106 SIM S/N MP 4259 DMT 117106 SIM MP4259 Tubes Breath Tubes Keyboard X Other: Power Cords	Radar: Control Unit Antenna(s) Antenna Cable(s) Power Cord Forks Other:	<i>* Breath tube</i> <i>* Simulator tube</i>
I acknowledge I am signing this Service Authorization Form as an act and deed of said agency, organization, or municipality, and that I am duly authorized to sign same for the uses and purposes mentioned herein. <b>PLEASE SIGN AND DATE.</b>		
Signature 		Date 05/25/2023

**DCJS USE ONLY**

*Inspected instrument, checked setup voltages, print and remote operation. Performed calibration/adjustment procedure, ran subject technician + diagnostic tests, verified calibration. \* 5-25-2023*