



**CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS
MAINTAINED IN THE REGULAR COURSE OF BUSINESS**

I, Frank Sgarlata, Highway Safety Equipment Technician 2, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NATL PATENT ANALYTICAL SYSTEM, DATAMASTER DMT breath test instrument, serial number 117106, performed on May 07, 2024 by Office of Public Safety employee Martin Schilling, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance /calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink that reads "Frank Sgarlata".

Digitally signed under ESRA
by Frank Sgarlata
on 05/08/2024 11:33 AM

**Frank Sgarlata
Highway Safety Equipment Technician 2
Office of Public Safety**

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Glens Falls City Police Department

Manufacturer: NATL PATENT ANALYTICAL SYSTEM

Model: DATAMASTER DMT

Serial Number: 117106

Date: May 07, 2024

Reference Solution Lot Number : 23451

Reference Solution Standard : 0.10% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.099 %	34.02 degrees centigrade
2	0.098 %	34.01 degrees centigrade
3	0.099 %	34.02 degrees centigrade
4	0.099 %	34.01 degrees centigrade

Reference Solution Lot Number : 24011

Reference Solution Standard : 0.08% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.080 %	34.02 degrees centigrade
2	0.079 %	34.01 degrees centigrade
3	0.079 %	34.01 degrees centigrade
4	0.079 %	34.02 degrees centigrade

Reference Solution Lot Number : 23380


Reference Solution Standard : 0.18% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.177 %	34.02 degrees centigrade
2	0.177 %	34.02 degrees centigrade
3	0.176 %	34.02 degrees centigrade
4	0.177 %	34.01 degrees centigrade

I hereby certify that I have performed any necessary maintenance procedures and calibrated NATL PATENT ANALYTICAL SYSTEM breath test instrument model DATAMASTER DMT, serial number 117106, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.

I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.

Performed by:

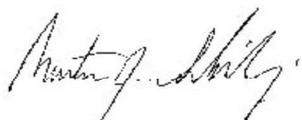

Digitally signed under ESRA
by Martin Schilling
on 05/07/2024 02:44 PM

Reviewed by:



Digitally signed under ESRA
by Jonathan Mascolo
on 05/07/2024 03:03 PM

Martin Schilling
Highway Safety Equipment Technician
Breath Analysis Operator Permit #45926

Jonathan Mascolo
Breath Analysis Technical Supervisor

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Glens Falls City Police Department
Manufacturer: NATL PATENT ANALYTICAL SYSTEM
Model: DATAMASTER DMT
Serial Number: 117106
Date: May 07, 2024

- 1. General appearance and condition of this device -----: **OK**

- 2. Check controls and indicators -----: **OK**

- 3. Check breath flow system -----: **OK**

- 4. Check printer operation -----: **OK**

- 5. System cycles through all modes -----: **OK**



6. Record any repairs made to this instrument and list services provided : INSPECTED INSTRUMENT, CHECKED SETUP VOLTAGES PRINT AND REMOTE OPERATION. PERFORMED CALIBRATION/ADJUSTMENT PROCEDURE, RAN SUBJECT, TECHNICIAN AND DIAGNOSTIC TESTS, VERIFIED CALIBRATION.

THIS CERTIFICATE EXPIRES 365 DAYS FROM THE DATE AT THE TOP OF THIS PAGE.

Performed by:

Digitally signed under ESRA
by Martin Schilling
on 05/07/2024 02:44 PM

Reviewed by:

Digitally signed under ESRA
by Jonathan Mascolo
on 05/07/2024 03:03 PM

Martin Schilling
Highway Safety Equipment Technician
Breath Analysis Operator Permit #45926

Jonathan Mascolo
Breath Analysis Technical Supervisor

TECHNICIAN TEST

GLENS FALLS CITY
POLICE DEPT
DATAMASTER dmt: 117106


Date: 05/07/2024

OPERATOR NAME:
MARTIN J SCHILLING
Permit #: 45926
Operator Agency/Dept: GLENS FALLS CITY PD
Reference Standard #: 24011

Nominal = 0.080 g/210L

BLANK TEST	0.000	14:01
INTERNAL STANDARD	VERIFIED	14:01
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.080	14:02
BLANK TEST	0.000	14:03
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.079	14:03
BLANK TEST	0.000	14:04
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.079	14:04
BLANK TEST	0.000	14:05
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.079	14:05
BLANK TEST	0.000	14:06

Average = 0.0792
Std Dev = 0.0005

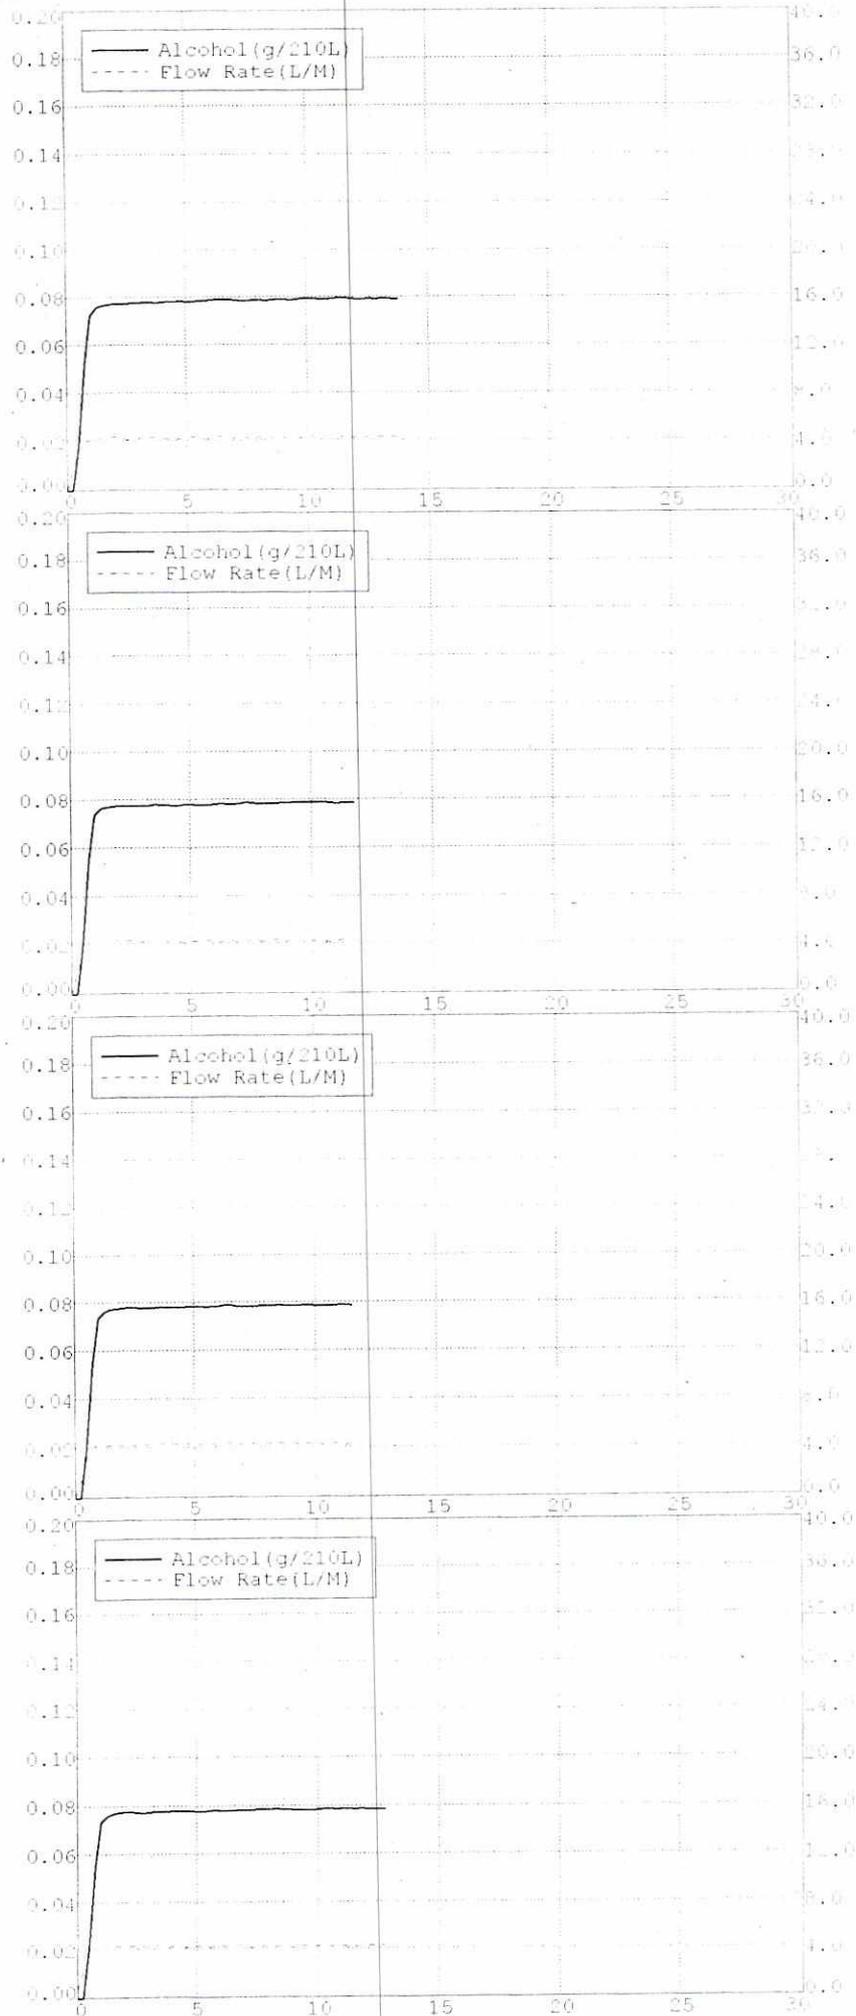

TECHNICIAN TEST

 GLENS FALLS CITY
 POLICE DEPT
 DATAMASTER dmt: 117106





Date: 05/07/2024

OPERATOR NAME:
 MARTIN J SCHILLING
 Permit #: 45926
 Operator Agency/Dept: GLENS FALLS CITY PD
 Reference Standard #: 23451

Nominal = 0.100 g/210L

BLANK TEST	0.000	12:19
INTERNAL STANDARD	VERIFIED	12:19
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.099	12:19
BLANK TEST	0.000	12:20
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.098	12:21
BLANK TEST	0.000	12:21
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.099	12:22
BLANK TEST	0.000	12:23
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.099	12:23
BLANK TEST	0.000	12:24

Average = 0.0988
 Std Dev = 0.0005

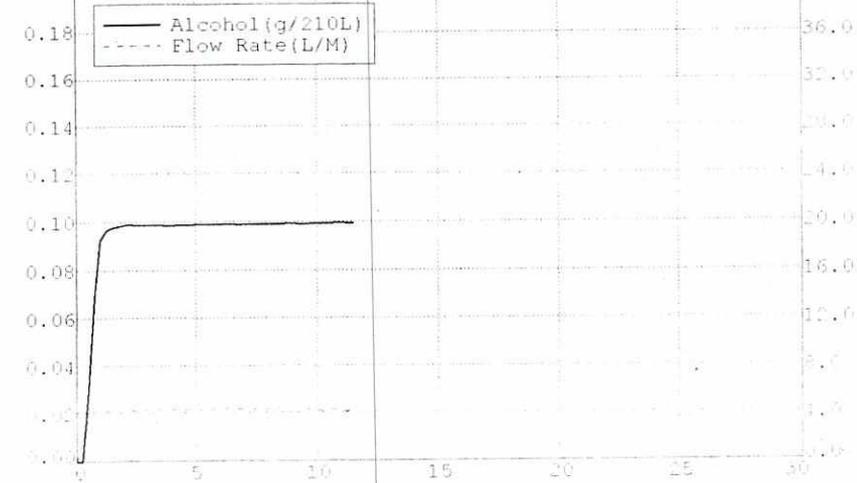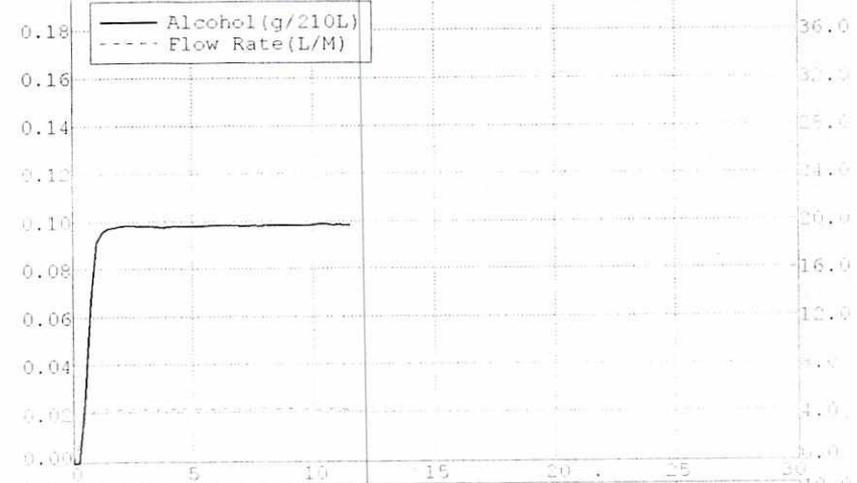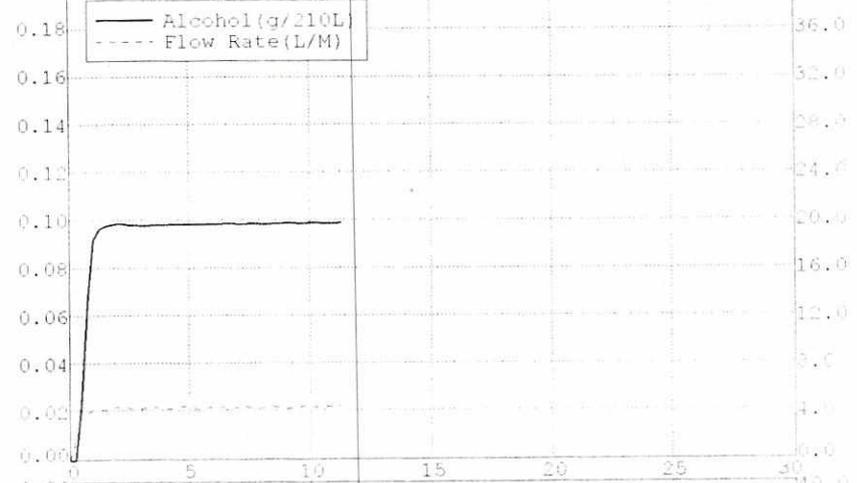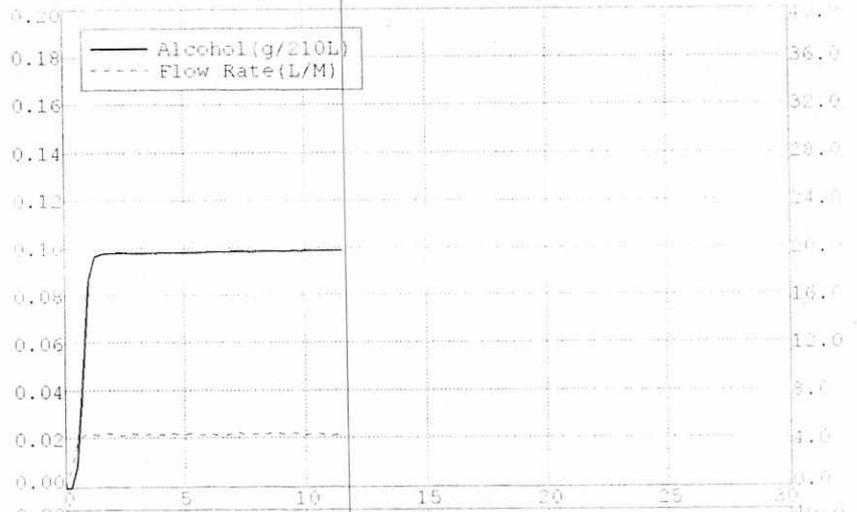

TECHNICIAN TEST

 GLENS FALLS CITY
 POLICE DEPT
 DATAMASTER dmt: 117106





Date: 05/07/2024

OPERATOR NAME:
 MARTIN J SCHILLING
 Permit #: 45926
 Operator Agency/Dept: GLENS FALLS CITY PD
 Reference Standard #: 23380

Nominal = 0.180 g/210L

BLANK TEST	0.000	14:30
INTERNAL STANDARD	VERIFIED	14:30
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.177	14:31
BLANK TEST	0.000	14:32
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.177	14:32
BLANK TEST	0.000	14:33
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.176	14:34
BLANK TEST	0.000	14:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.177	14:35
BLANK TEST	0.000	14:36

Average = 0.1768
 Std Dev = 0.0005

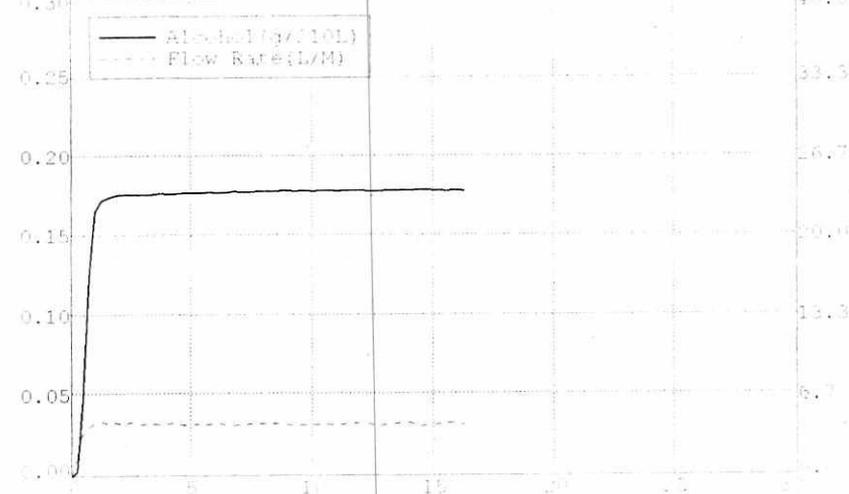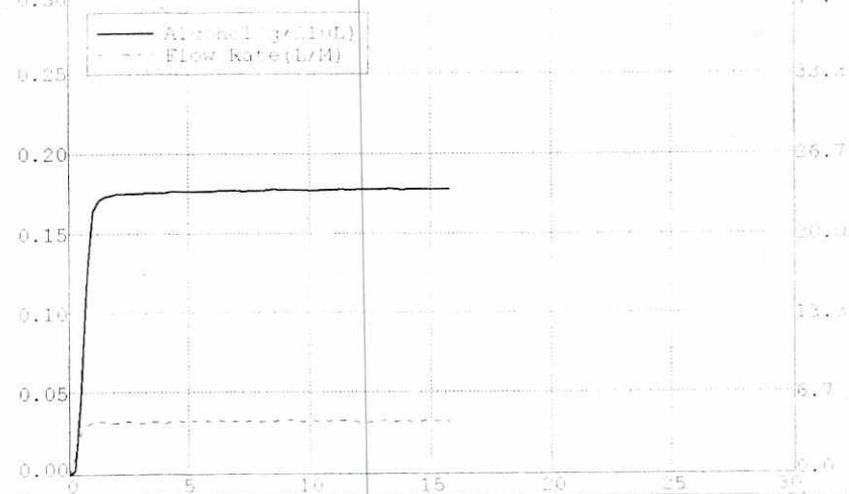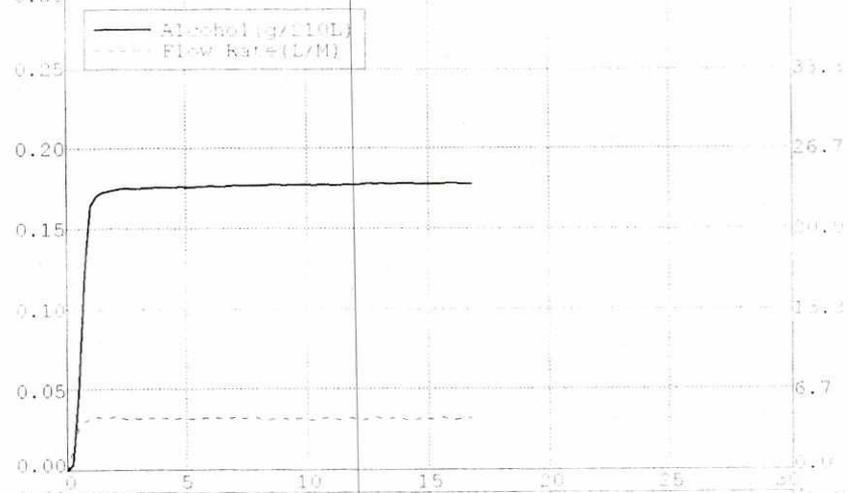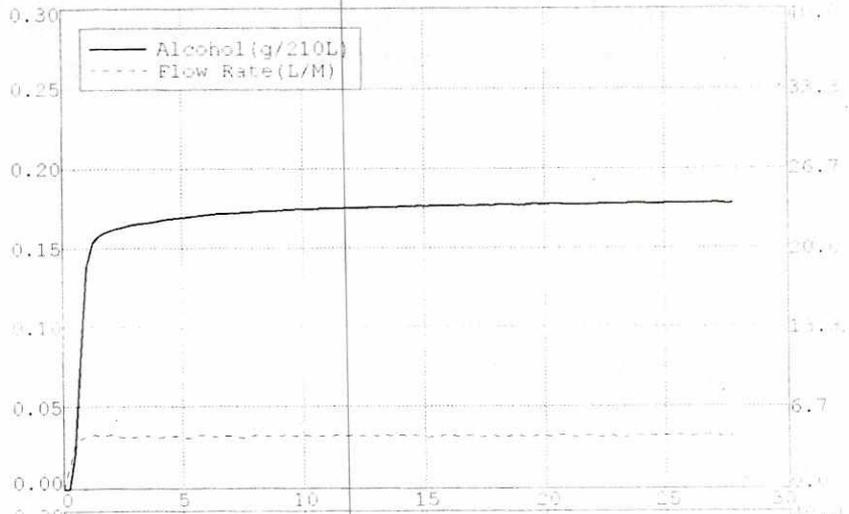

SERVICE AUTHORIZATION FORM
Highway Safety Technology Unit
80 South Swan Street
Albany, NY 12210
Ph: 518-485-7636 / 518-402-0689
Fax: 518-457-6869

My
5/2/24

THIS FORM IS USED TO AUTHORIZE THE DIVISION OF CRIMINAL JUSTICE SERVICES TO PERFORM SERVICE ON THE INSTRUMENT IDENTIFIED. THIS AUTHORIZATION MUST ACCOMPANY EACH PIECE OF EQUIPMENT WHEN IT IS PRESENTED TO THE EQUIPMENT REPAIR CENTER FOR SERVICE. **PLEASE SIGN AND DATE FORM.**

SECTION I - AGENCY INFORMATION

Name of Agency Glens Falls Police Department		Today's Date 05/07/2024
Address 42 Ridge Street		City, State, ZIP Glens Falls, New York 12801
Contact Person Lt. Ryan S. Pedone		Contact Telephone (518) 769-0596
Contact Email rpedone@glensfallspd.com		Best Way to Reach You During Appointment Period (518) 769-0596

SECTION II - INSTRUMENT INFORMATION

Instrument Manufacturer (Please Circle) NPAS DMT GUTH Applied Concepts (Stalker) Decatur (Genesis) Kustom (Eagle/Falcon) MPH Alco-Sensor Other:		
Model Number Datamaster DMT		Instrument Serial Number 117106
Antenna Serial Number (if applicable) Antenna 1 -- / Antenna 2 --		Type of maintenance (check appropriate) <input checked="" type="checkbox"/> Calibration Check <input type="checkbox"/> Repair
Brief Description of Malfunction Yearly Calibration Check		
List all parts, cables and/or accessories being submitted. Tuning forks must accompany all radar units (if applicable). (Please Circle)		
DMT/SIM: DMT <input checked="" type="checkbox"/> SIM Keyboard <input checked="" type="checkbox"/> Other: <input checked="" type="checkbox"/> Power cord		Radar: Control Unit Antenna(s) Antenna Cable(s) Power Cord Forks Other:
I acknowledge I am signing this Service Authorization Form as an act and deed of said agency, organization, or municipality, and that I am duly authorized to sign same for the uses and purposes mentioned herein. PLEASE SIGN AND DATE.		
Signature <i>[Signature]</i> 45757		Date 05/07/2024

DCJS USE ONLY

*In requested instrument. Checked return to repair center.
 performed calibration/adjustment procedure. For subject, technician and supervisor
 test. Verified calibration*