



**CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS
MAINTAINED IN THE REGULAR COURSE OF BUSINESS**

I, Frank Sgarlata, Highway Safety Equipment Technician 2, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NATL PATENT ANALYTICAL SYSTEM, DATAMASTER DMT breath test instrument, serial number 117106, performed on October 16, 2024 by Office of Public Safety employee Martin Schilling, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/ maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance /calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink that reads "Frank Sgarlata".

Digitally signed under ESRA
by Frank Sgarlata
on 10/17/2024 06:51 AM

**Frank Sgarlata
Highway Safety Equipment Technician 2
Office of Public Safety**

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Glens Falls City Police Department

Manufacturer: NATL PATENT ANALYTICAL SYSTEM

Model: DATAMASTER DMT

Serial Number: 117106

Date: October 16, 2024

Reference Solution Lot Number : 23451

Reference Solution Standard : 0.10% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.101 %	34.00 degrees centigrade
2	0.099 %	34.01 degrees centigrade
3	0.100 %	34.00 degrees centigrade
4	0.099 %	34.01 degrees centigrade

Reference Solution Lot Number : 24011

Reference Solution Standard : 0.08% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.079 %	34.01 degrees centigrade
2	0.079 %	34.00 degrees centigrade
3	0.079 %	34.01 degrees centigrade
4	0.079 %	34.00 degrees centigrade

Reference Solution Lot Number : 24290


Reference Solution Standard : 0.18% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.176 %	34.01 degrees centigrade
2	0.176 %	34.01 degrees centigrade
3	0.177 %	34.01 degrees centigrade
4	0.177 %	34.00 degrees centigrade

I hereby certify that I have performed any necessary maintenance procedures and calibrated NATL PATENT ANALYTICAL SYSTEM breath test instrument model DATAMASTER DMT, serial number 117106, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.

I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.

Performed by:



Digitally signed under ESRA
by Martin Schilling
on 10/16/2024 02:32 PM

Reviewed by:



Digitally signed under ESRA
by Jonathan Mascolo
on 10/16/2024 02:57 PM

Martin Schilling
Highway Safety Equipment Technician
Breath Analysis Operator Permit #45926

Jonathan Mascolo
Breath Analysis Technical Supervisor

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Glens Falls City Police Department
Manufacturer: NATL PATENT ANALYTICAL SYSTEM
Model: DATAMASTER DMT
Serial Number: 117106
Date: October 16, 2024

1. General appearance and condition of this device -----: Customer stated simulator times out.

2. Check controls and indicators -----: OK

3. Check breath flow system -----: OK

4. Check printer operation -----: OK

5. System cycles through all modes -----: OK



6. Record any repairs made to this instrument and list services provided : CLEANED 5WAY VALVE AND REPLACED DETECTOR. INSPECTED INSTRUMENT, CHECKED SETUP VOLTAGES PRINT AND REMOTE OPERATION. PERFORMED CALIBRATION/ADJUSTMENT PROCEDURE, RAN SUBJECT, TECHNICIAN AND DIAGNOSTIC TESTS, VERIFIED CALIBRATION.

THIS CERTIFICATE EXPIRES 365 DAYS FROM THE DATE AT THE TOP OF THIS PAGE.

Performed by:

Digitally signed under ESRA
by Martin Schilling
on 10/16/2024 02:32 PM

Reviewed by:

Digitally signed under ESRA
by Jonathan Mascolo
on 10/16/2024 02:57 PM

Martin Schilling
Highway Safety Equipment Technician
Breath Analysis Operator Permit #45926

Jonathan Mascolo
Breath Analysis Technical Supervisor

TECHNICIAN TEST

GLENS FALLS CITY
POLICE DEPT
DATAMASTER dmt: 117106

Date: 10/16/2024





OPERATOR NAME:
MARTIN J SCHILLING
Permit #: 45926
Operator Agency/Dept: GLENS FALLS CITY PD
Reference Standard #: 24011

Nominal = 0.080 g/210L

BLANK TEST	0.000	10:36
INTERNAL STANDARD	VERIFIED	10:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.079	10:37
BLANK TEST	0.000	10:37
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.079	10:38
BLANK TEST	0.000	10:39
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.079	10:39
BLANK TEST	0.000	10:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.079	10:40
BLANK TEST	0.000	10:41

Average = 0.0790

Std Dev = 0.0000

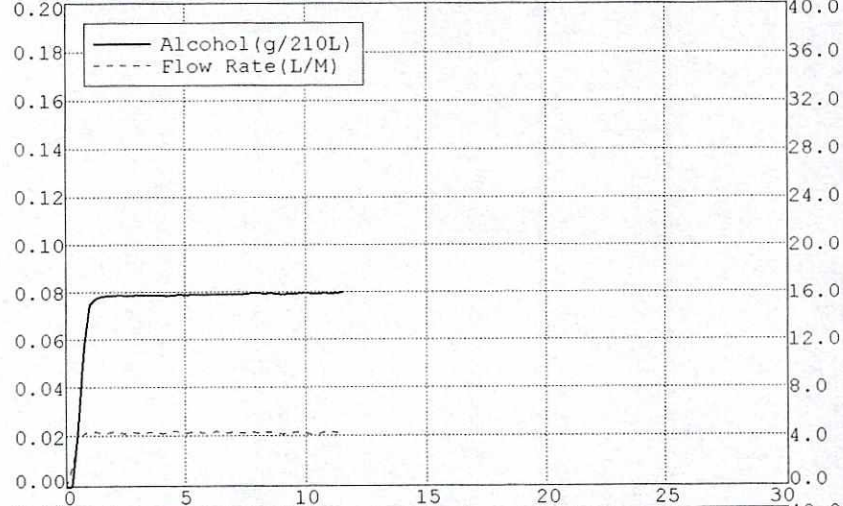

TECHNICIAN TEST

 GLENS FALLS CITY
 POLICE DEPT
 DATAMASTER dmt: 117106





Date: 10/16/2024

OPERATOR NAME:
 MARTIN J SCHILLING
 Permit #: 45926
 Operator Agency/Dept: GLENS FALLS CITY PD
 Reference Standard #: 23451

Nominal = 0.100 g/210L

BLANK TEST	0.000	08:56
INTERNAL STANDARD	VERIFIED	08:56
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.101	08:57
BLANK TEST	0.000	08:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.099	08:58
BLANK TEST	0.000	08:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.100	08:59
BLANK TEST	0.000	09:00
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.099	09:01
BLANK TEST	0.000	09:01

Average = 0.0998
 Std Dev = 0.0010

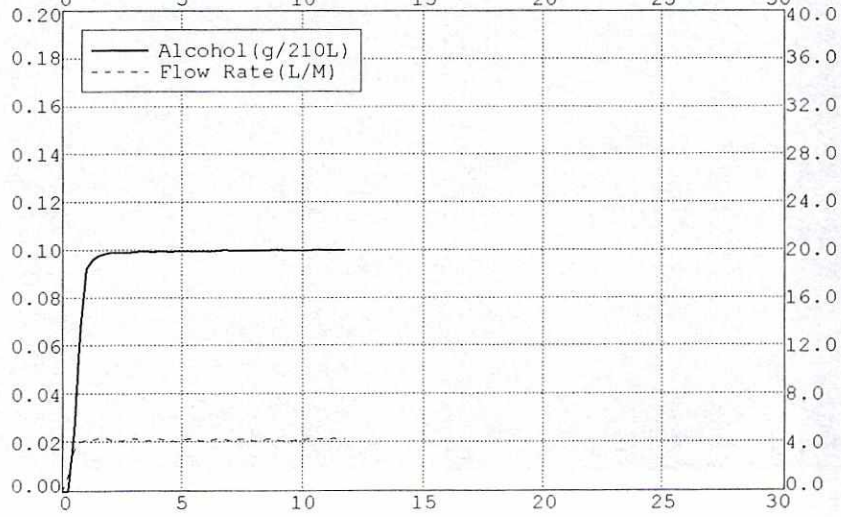

TECHNICIAN TEST

 GLENS FALLS CITY
 POLICE DEPT
 DATAMASTER dmt: 117106




Date: 10/16/2024

OPERATOR NAME:
 MARTIN J SCHILLING
 Permit #: 45926
 Operator Agency/Dept: GLENS FALLS CITY PD
 Reference Standard #: 24290

Nominal = 0.180 g/210L

BLANK TEST	0.000	10:52
INTERNAL STANDARD	VERIFIED	10:52
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.176	10:53
BLANK TEST	0.000	10:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.176	10:54
BLANK TEST	0.000	10:55
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.177	10:55
BLANK TEST	0.000	10:56
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.177	10:57
BLANK TEST	0.000	10:58

Average = 0.1765
 Std Dev = 0.0006



DJ
10.16.24

SERVICE AUTHORIZATION FORM
Highway Safety Technology Unit
80 South Swan Street
Albany, NY 12210
Ph: 518-485-7636 / 518-402-0689
Fax: 518-457-6869

THIS FORM IS USED TO AUTHORIZE THE DIVISION OF CRIMINAL JUSTICE SERVICES TO PERFORM SERVICE ON THE INSTRUMENT IDENTIFIED. THIS AUTHORIZATION MUST ACCOMPANY EACH PIECE OF EQUIPMENT WHEN IT IS PRESENTED TO THE EQUIPMENT REPAIR CENTER FOR SERVICE. **PLEASE SIGN AND DATE FORM.**

SECTION I - AGENCY INFORMATION

Name of Agency Glens Falls Police Department		Today's Date 09/17/2024
Address 42 Ridge Street		City, State, ZIP Glens Falls, New York 12801
Contact Person Lt. Ryan S. Pedone		Contact Telephone (518) 769-0596
Contact Email rpedone@glensfallspd.com		Best Way to Reach You During Appointment Period (518) 769-0596

SECTION II - INSTRUMENT INFORMATION

Instrument Manufacturer (Please Circle) NPAS DMT GUTH Applied Concepts (Stalker) Decatur (Genesis) Kustom (Eagle/Falcon) MPH Alco-Sensor Other:		
Model Number Datamaster DMT		Instrument Serial Number 117106
Antenna Serial Number (if applicable) Antenna 1 -- / Antenna 2 --		Type of maintenance (check appropriate) <input type="checkbox"/> Calibration Check <input checked="" type="checkbox"/> Repair
Brief Description of Malfunction Simulator Times out when using Happened multiple times on 9/16/2024 and once 9/17/2024		
List all parts, cables and/or accessories being submitted. Tuning forks must accompany all radar units (if applicable). (Please Circle)		
DMT/SIM: DMT SIM Tubes Keyboard yes Other: Power Cord		Radar: Control Unit Antenna(s) Antenna Cable(s) Power Cord Forks Other: _
<i>I acknowledge I am signing this Service Authorization Form as an act and deed of said agency, organization, or municipality, and that I am duly authorized to sign same for the uses and purposes mentioned herein. PLEASE SIGN AND DATE.</i>		
Signature 65757		Date 09/17/2024

DCJS USE ONLY

<p><i>Cleaned 5 way valve and replaced detector. Inspected instrument. Checked petra voltages front and remote operation. Performed calibration / adjustment procedure, for subject, tubes and diagnostic test. Verified calibration.</i></p>
