

SUPERVISOR TEST




GLENS FALLS CITY
POLICE DEPT
DATAMASTER dmt: 117106

Date: 10/14/2019

OPERATOR NAME:
SHAWN A LOVELACE
Permit #: 30657
Operator Agency/Dept: GLENS FALLS CITY PD
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:16
INTERNAL STANDARD	VERIFIED	07:16
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	07:16
BLANK TEST	0.00	07:17
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	07:18
BLANK TEST	0.00	07:18
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	07:19
BLANK TEST	0.00	07:20

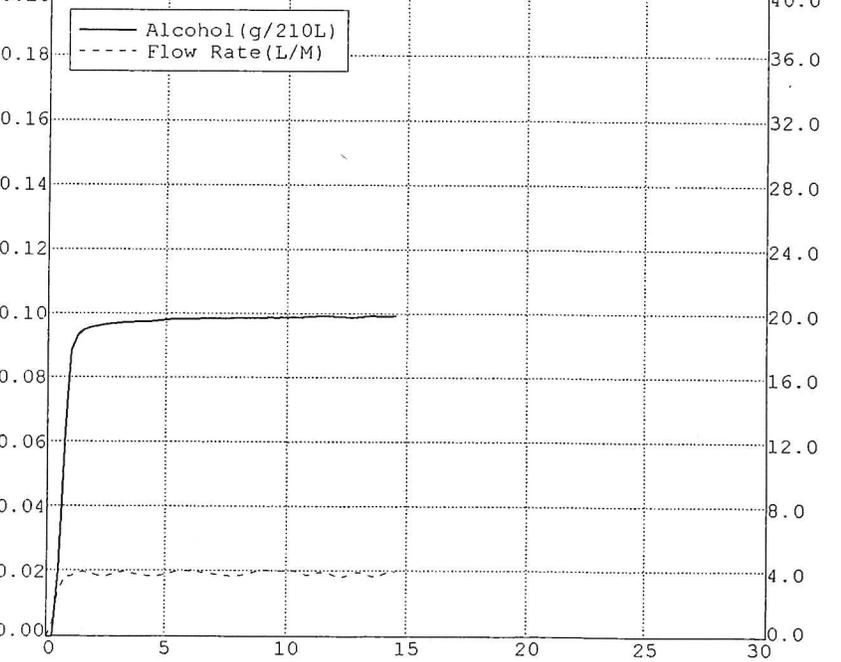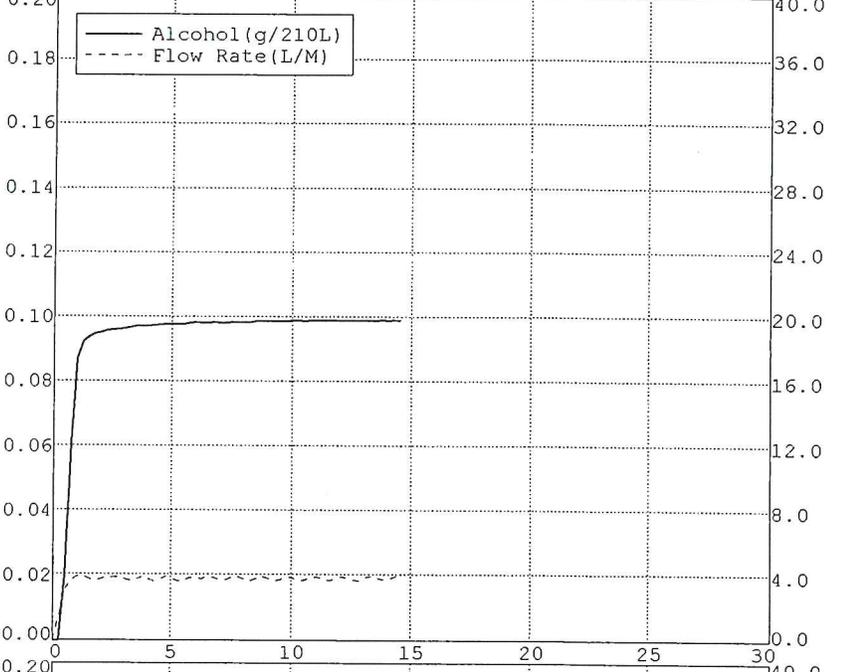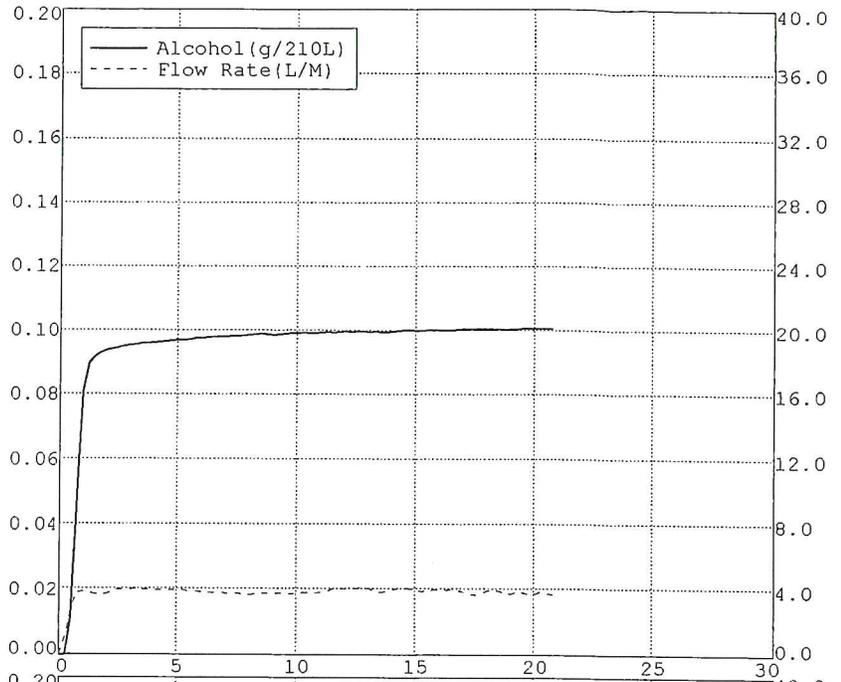

SUPERVISOR TEST

GLENS FALLS CITY
POLICE DEPT
DATAMASTER dmt: 117106



Date: 10/14/2019

OPERATOR NAME:
TYLER R MELLO
Permit #: 46781
Operator Agency/Dept: GLENS FALLS CITY PD
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:20
INTERNAL STANDARD	VERIFIED	02:20
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	02:21
BLANK TEST	0.00	02:22
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	02:22

Blank Error

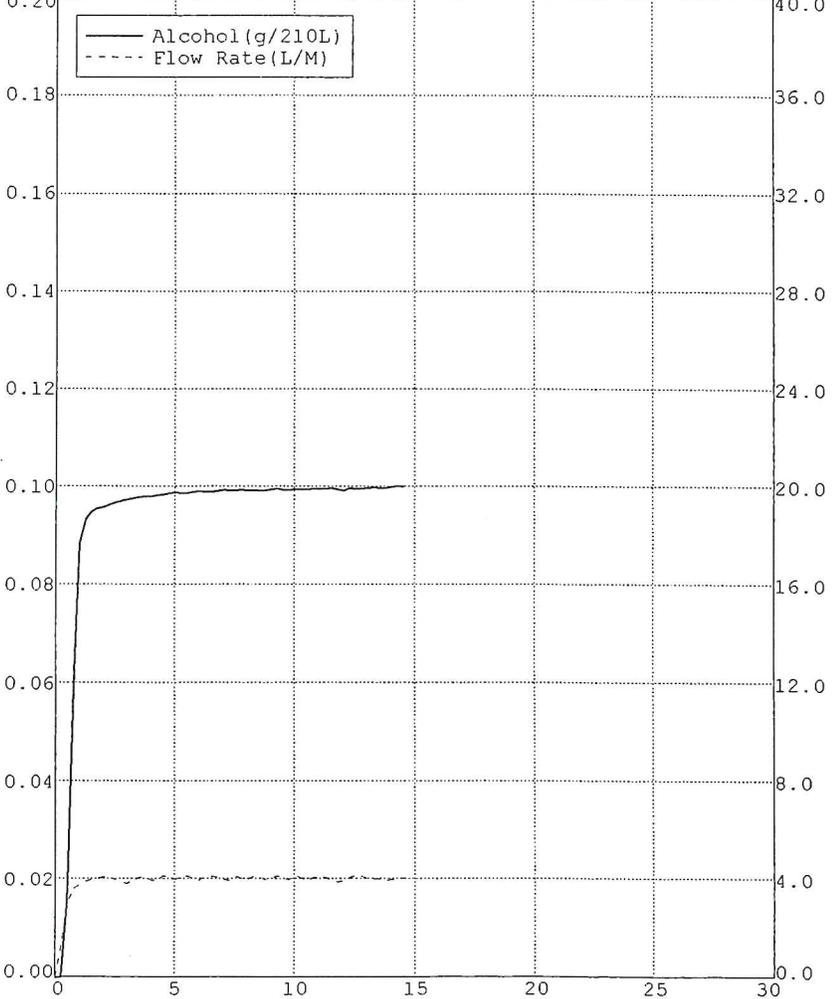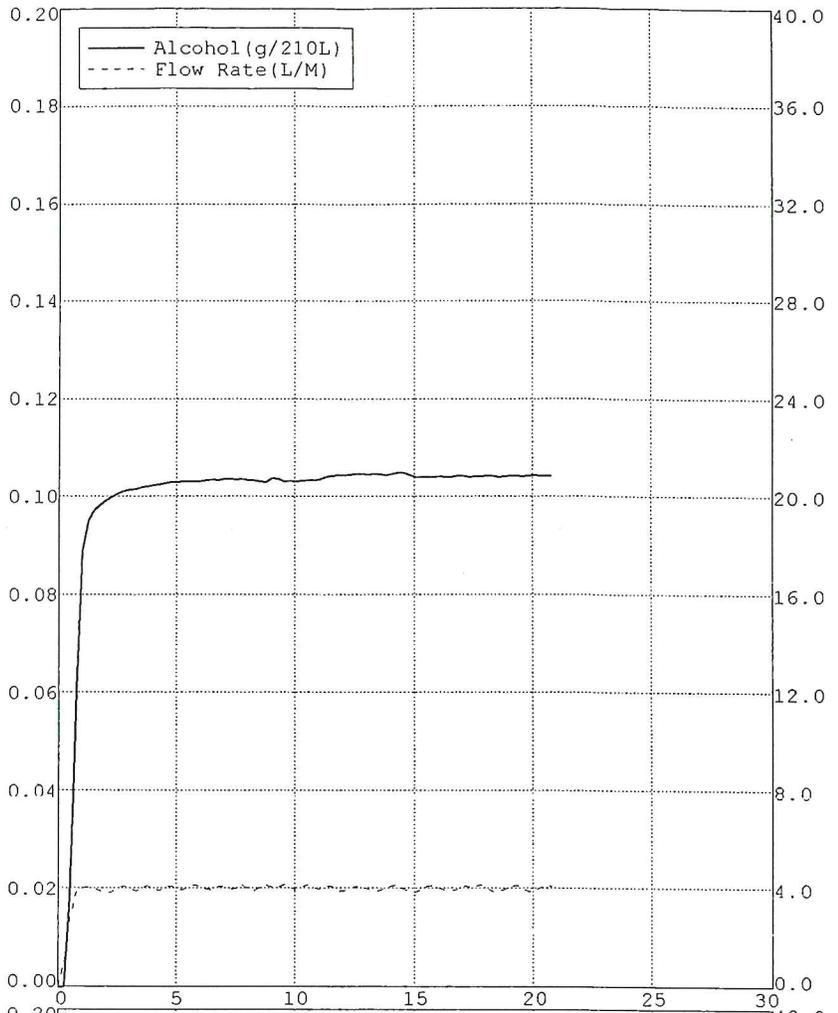

SUPERVISOR TEST

GLENS FALLS CITY
POLICE DEPT
DATAMASTER dmt: 117106

Date: 10/14/2019

OPERATOR NAME:
TYLER R MELLO
Permit #: 46781
Operator Agency/Dept: GLENS FALLS CITY PD
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:11
INTERNAL STANDARD	VERIFIED	02:11
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	02:12
BLANK TEST	0.00	02:13
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	02:13
BLANK TEST	0.00	02:14
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	02:14

Blank Error

