

SUPERVISOR TEST



-----  
GLENS FALLS CITY  
POLICE DEPT  
DATAMASTER dmt: 117106  
-----

Date: 02/10/2020

OPERATOR NAME:  
GERALD C WILLETTE  
Permit #: 32550  
Operator Agency/Dept: GLENS FALLS CITY PD  
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:13
INTERNAL STANDARD	VERIFIED	00:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:13
BLANK TEST	0.00	00:14
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	00:14
BLANK TEST	0.00	00:15
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:16
BLANK TEST	0.00	00:17

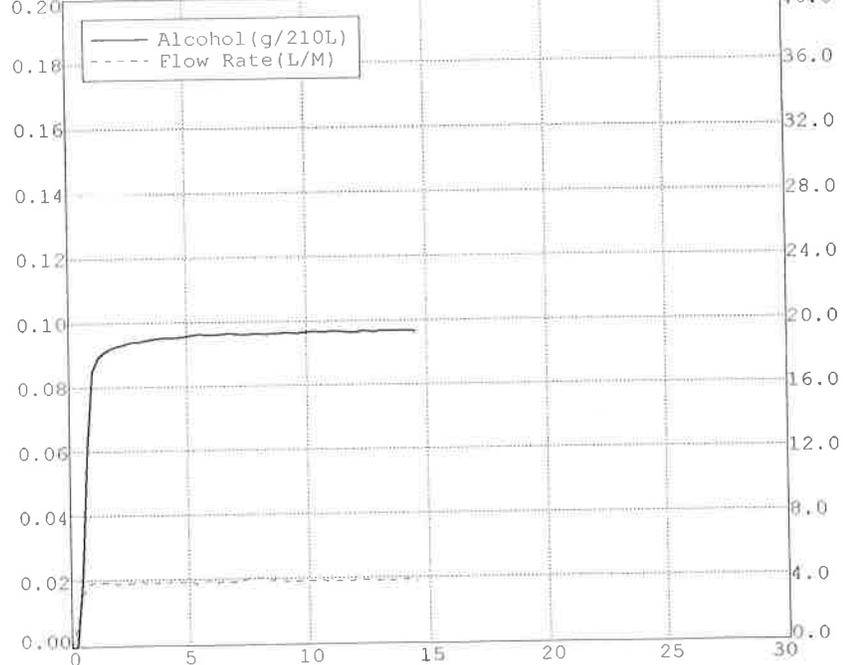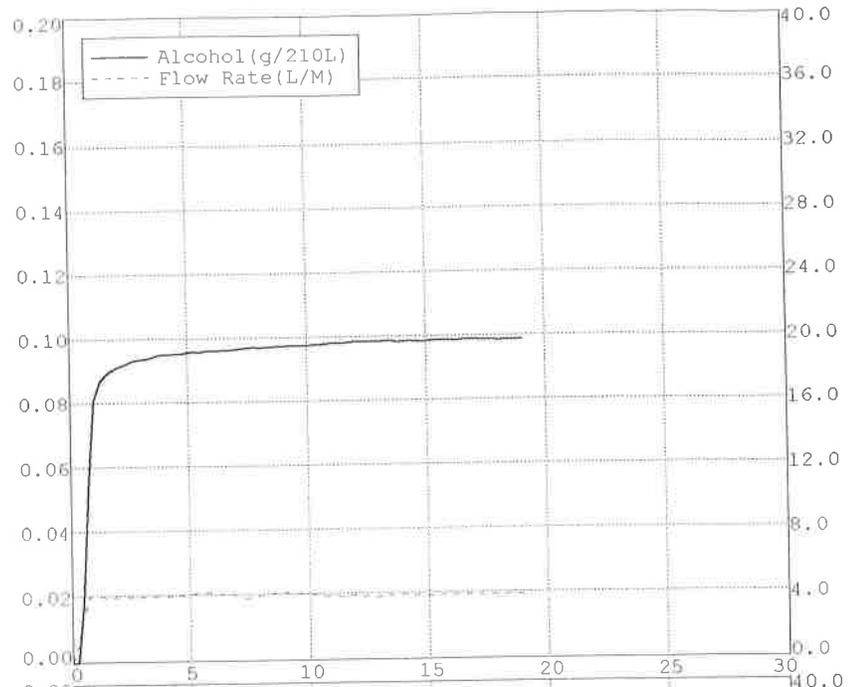

SUPERVISOR TEST

GLENS FALLS CITY  
POLICE DEPT  
DATAMASTER dmt: 117106

Date: 02/10/2020

OPERATOR NAME:  
GERALD C WILLETTE  
Permit #: 32550  
Operator Agency/Dept: GLENS FALLS CITY PD  
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:06
INTERNAL STANDARD	VERIFIED	00:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:07
BLANK TEST	0.00	00:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	00:08
BLANK TEST	0.00	00:09
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:09

Blank Error

