

SUPERVISOR TEST




GLENS FALLS CITY
 POLICE DEPT
 DATAMASTER dmt: 117106

Date: 03/30/2020

OPERATOR NAME:
 ROBERT M FOO
 Permit #: 46059
 Operator Agency/Dept: GLENS FALLS CITY PD
 Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:20
INTERNAL STANDARD	VERIFIED	00:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:21
BLANK TEST	0.00	00:22
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:22
BLANK TEST	0.00	00:23
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:23
BLANK TEST	0.00	00:24

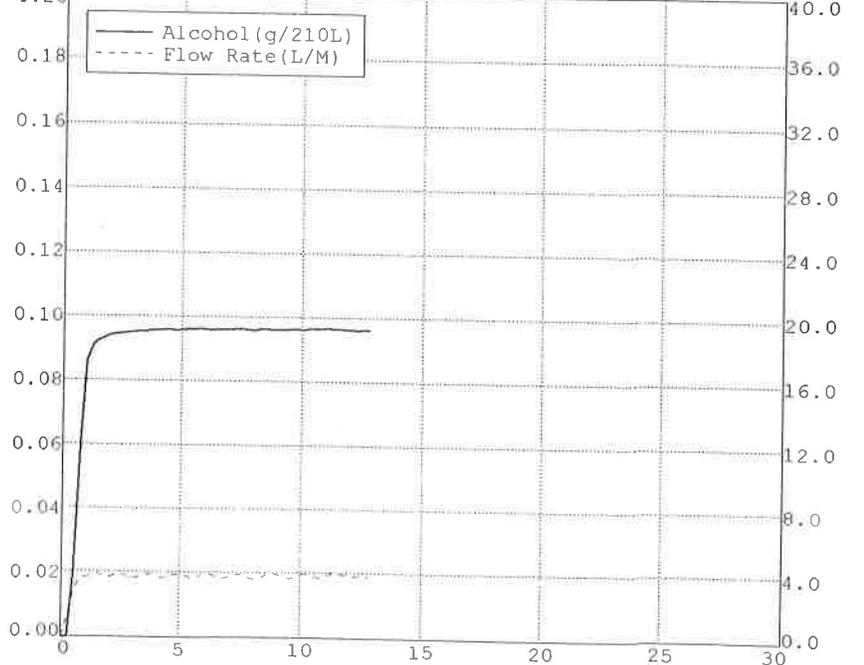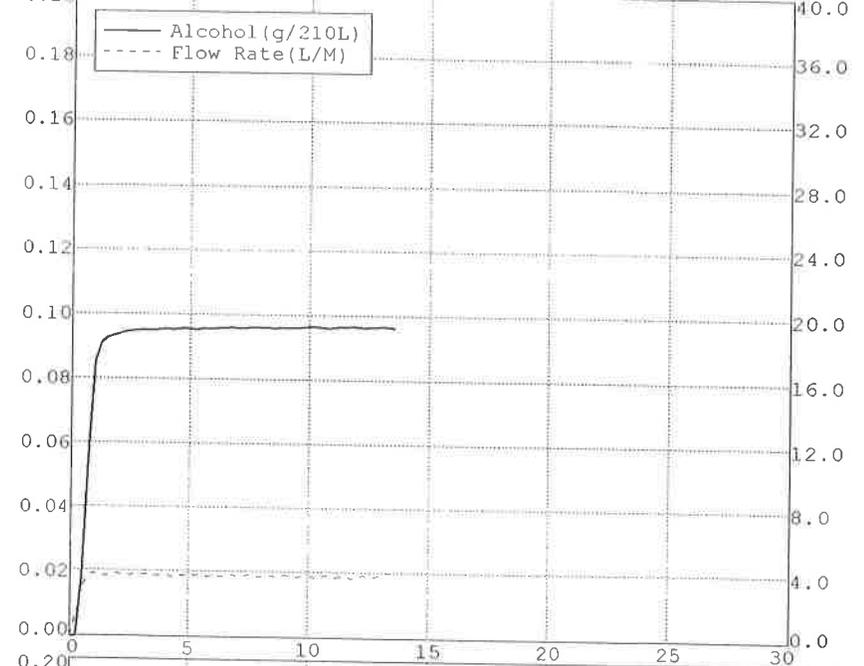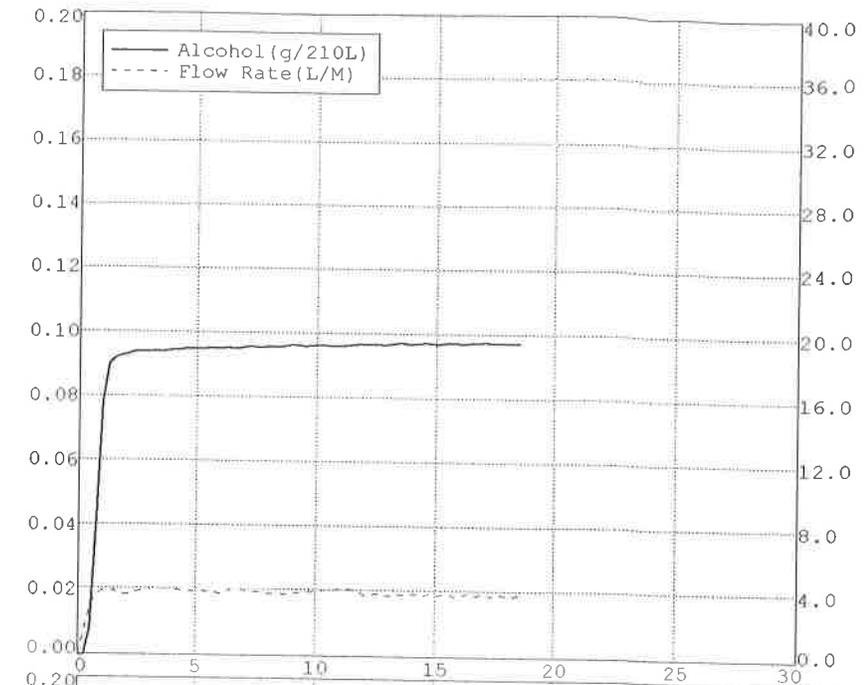

SOLUTION CHANGE




GLENS FALLS CITY
POLICE DEPT
DATAMASTER dmt: 117106

Date: 04/03/2020

OPERATOR NAME:
GERALD C WILLETTE
Permit #: 32550
Operator Agency/Dept: GLENS FALLS CITY PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:05
INTERNAL STANDARD	VERIFIED	05:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	05:06
BLANK TEST	0.00	05:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	05:08
BLANK TEST	0.00	05:09
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	05:10
BLANK TEST	0.00	05:11

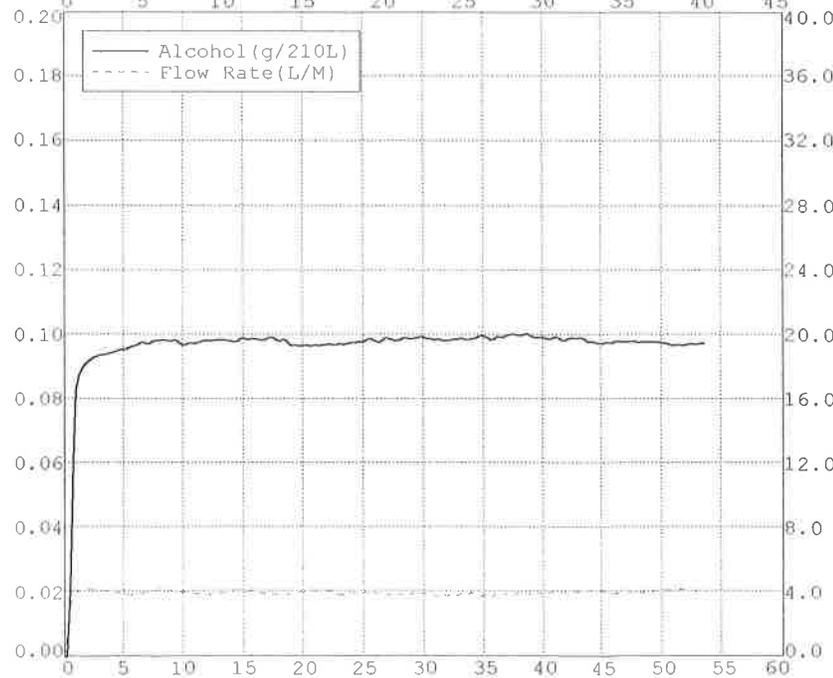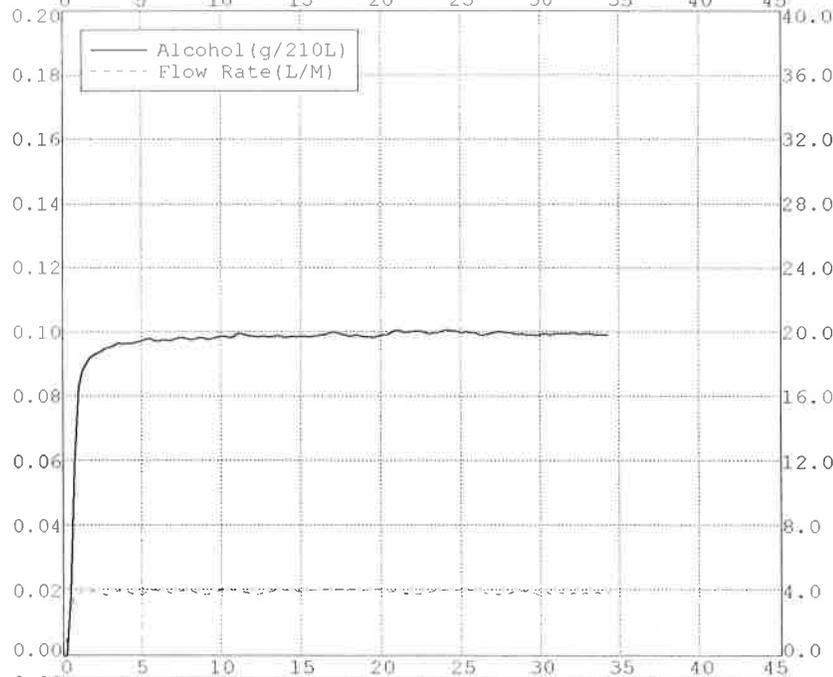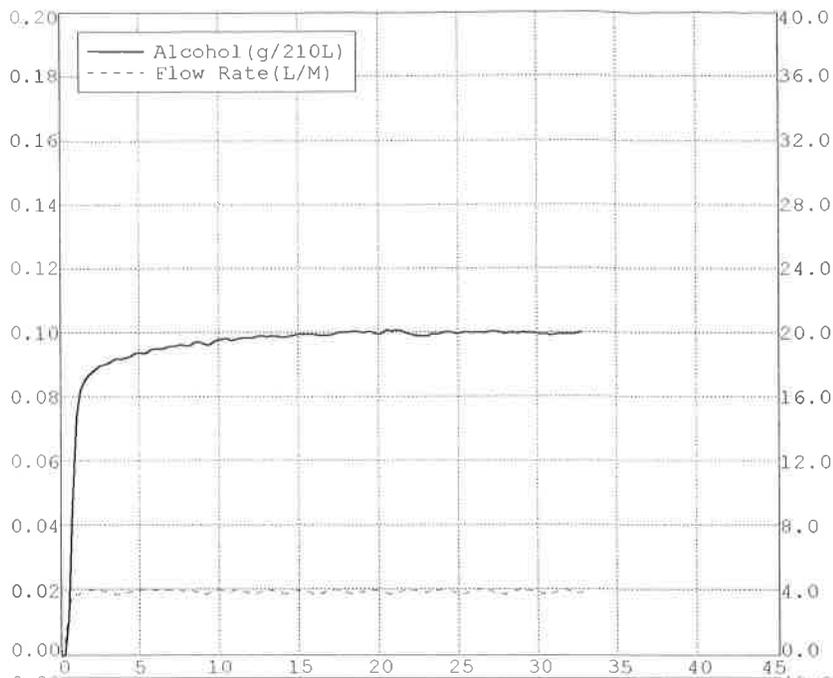

SOLUTION CHANGE

GLENS FALLS CITY
POLICE DEPT
DATAMASTER dmt: 117106

Date: 04/03/2020

OPERATOR NAME:
GERALD C WILLETTE
Permit #: 32550
Operator Agency/Dept: GLENS FALLS CITY PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:02
INTERNAL STANDARD	VERIFIED	04:02
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	04:03
BLANK TEST	0.00	04:04

Simulator Timed Out

