

SUPERVISOR TEST



 GLENS FALLS CITY
 POLICE DEPT
 DATAMASTER dmt: 117106

Date: 04/06/2020

OPERATOR NAME:
 ROBERT M FOO
 Permit #: 46059
 Operator Agency/Dept: GLENS FALLS CITY PD
 Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:13
INTERNAL STANDARD	VERIFIED	00:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:13
BLANK TEST	0.00	00:14
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:15
BLANK TEST	0.00	00:16
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:16
BLANK TEST	0.00	00:17

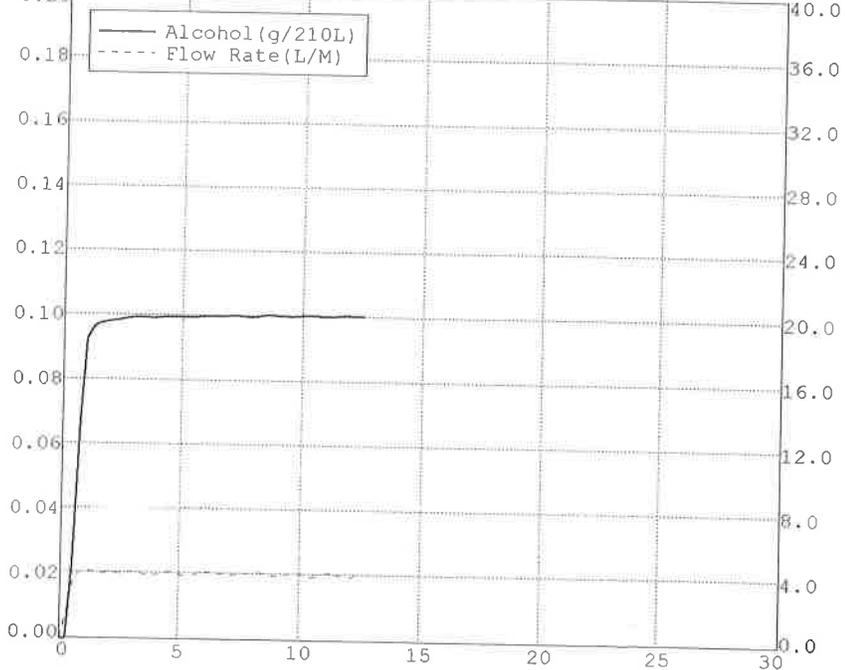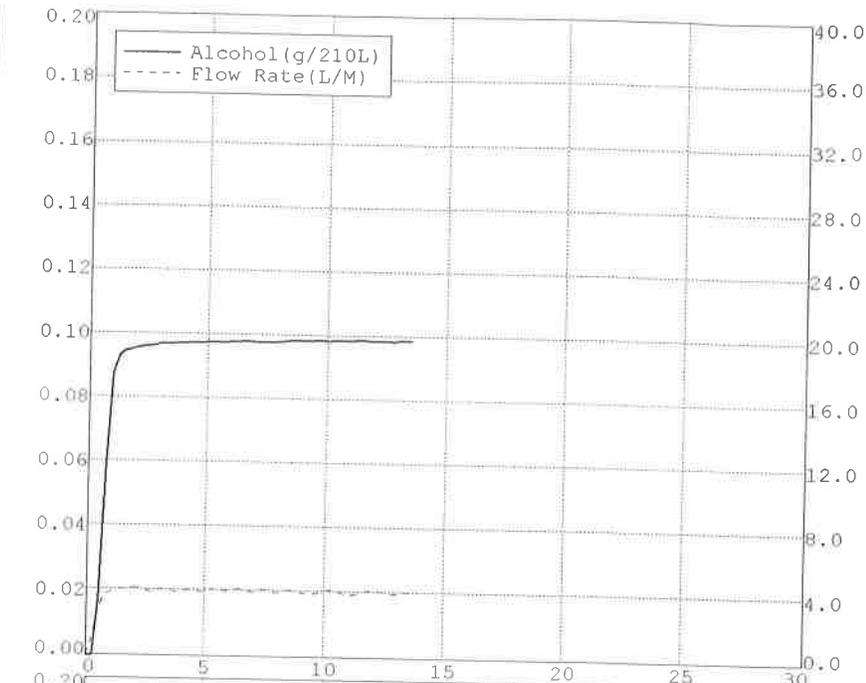

SUPERVISOR TEST

GLENS FALLS CITY
POLICE DEPT
DATAMASTER dmt: 117106


Date: 04/06/2020

OPERATOR NAME:
ROBERT M FOO
Permit #: 46059
Operator Agency/Dept: GLENS FALLS CITY PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:07
INTERNAL STANDARD	VERIFIED	00:07
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	INTERFERENCE	00:07

Interference Detected

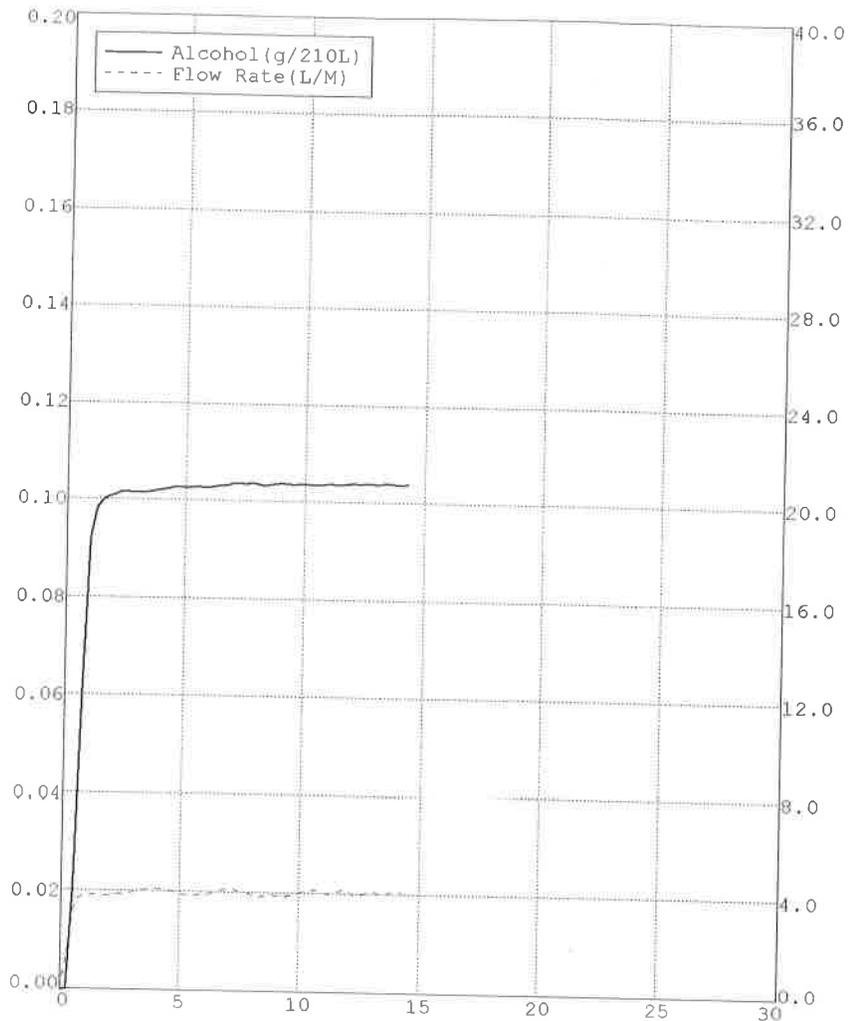

SUPERVISOR TEST

GLENS FALLS CITY
POLICE DEPT
DATAMASTER dmt: 117106

Date: 04/06/2020

OPERATOR NAME:
ROBERT M FOO
Permit #: 46059
Operator Agency/Dept: GLENS FALLS CITY PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:02
INTERNAL STANDARD	VERIFIED	00:02
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:02

Blank Error

