

SUPERVISOR TEST




-----  
GLENS FALLS CITY  
POLICE DEPT  
DATAMASTER dmt: 117106  
-----

Date: 04/27/2020

OPERATOR NAME:  
ROBERT M FOO  
Permit #: 46059  
Operator Agency/Dept: GLENS FALLS CITY PD  
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:34
INTERNAL STANDARD	VERIFIED	00:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:35
BLANK TEST	0.00	00:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:36
BLANK TEST	0.00	00:37
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:37
BLANK TEST	0.00	00:38

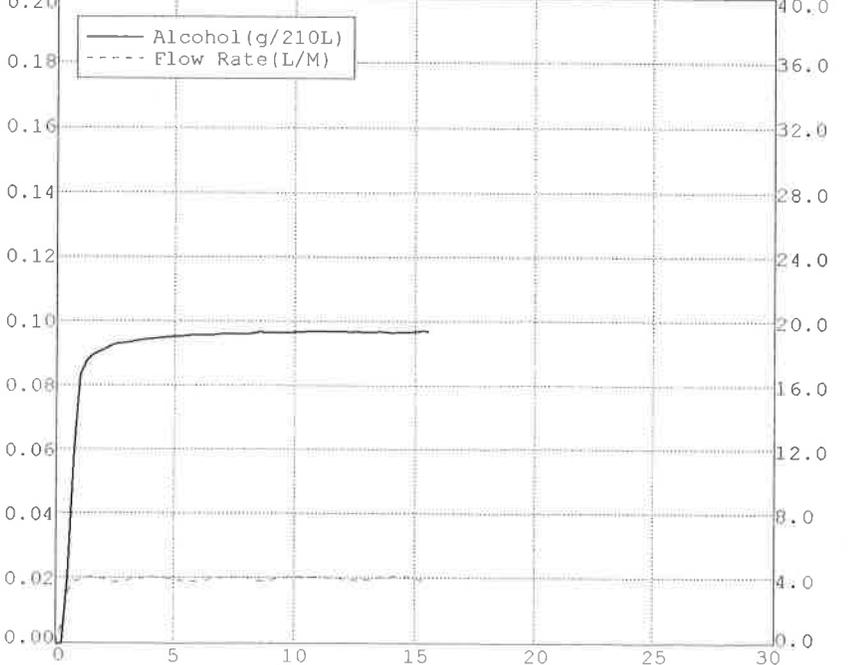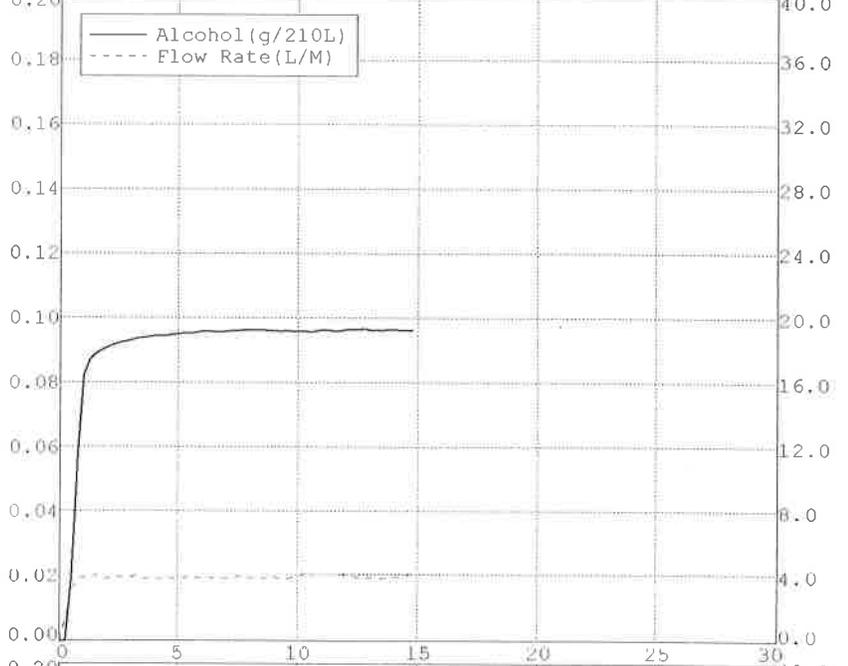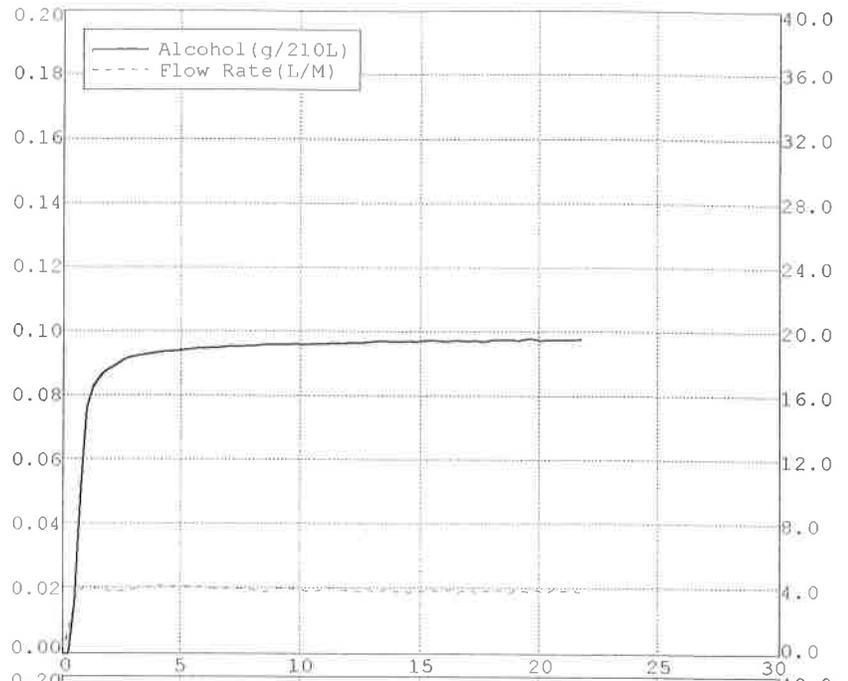

SUPERVISOR TEST

-----  
GLENS FALLS CITY  
POLICE DEPT  
DATAMASTER dmt: 117106  
-----

Date: 04/27/2020

OPERATOR NAME:  
ROBERT M FOO  
Permit #: 46059  
Operator Agency/Dept: GLENS FALLS CITY PD  
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:28
INTERNAL STANDARD	VERIFIED	00:29
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:29
BLANK TEST	0.00	00:30
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:30

Blank Error

