

SUPERVISOR TEST




GLENS FALLS CITY
POLICE DEPT
DATAMASTER dmt: 117106

Date: 06/08/2020

OPERATOR NAME:
THOMAS S PRATT
Permit #: 48766
Operator Agency/Dept: GLENS FALLS CITY PD
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:52
INTERNAL STANDARD	VERIFIED	00:53
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	00:53
BLANK TEST	0.00	00:54
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	00:54
BLANK TEST	0.00	00:55
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	00:55
BLANK TEST	0.00	00:56

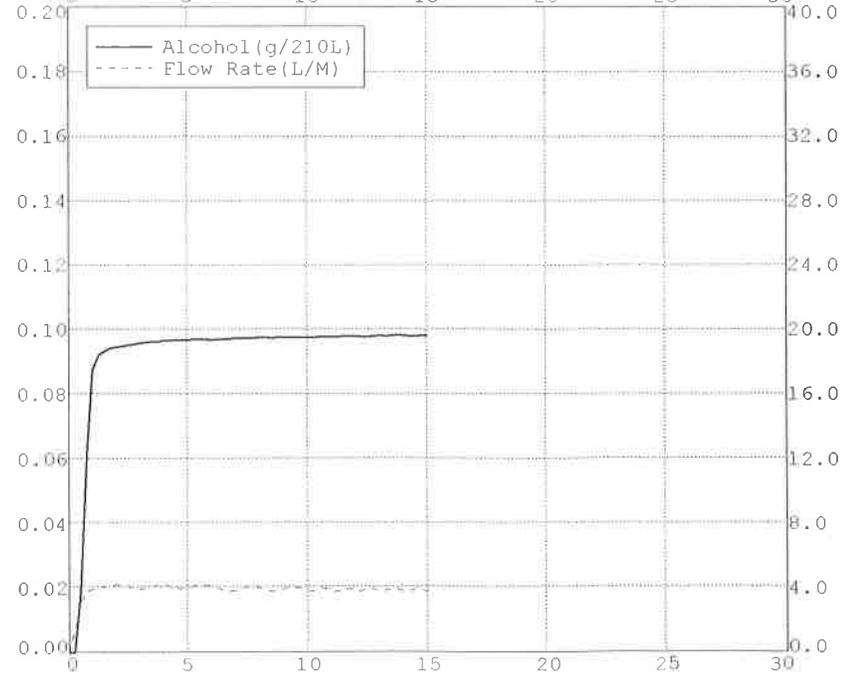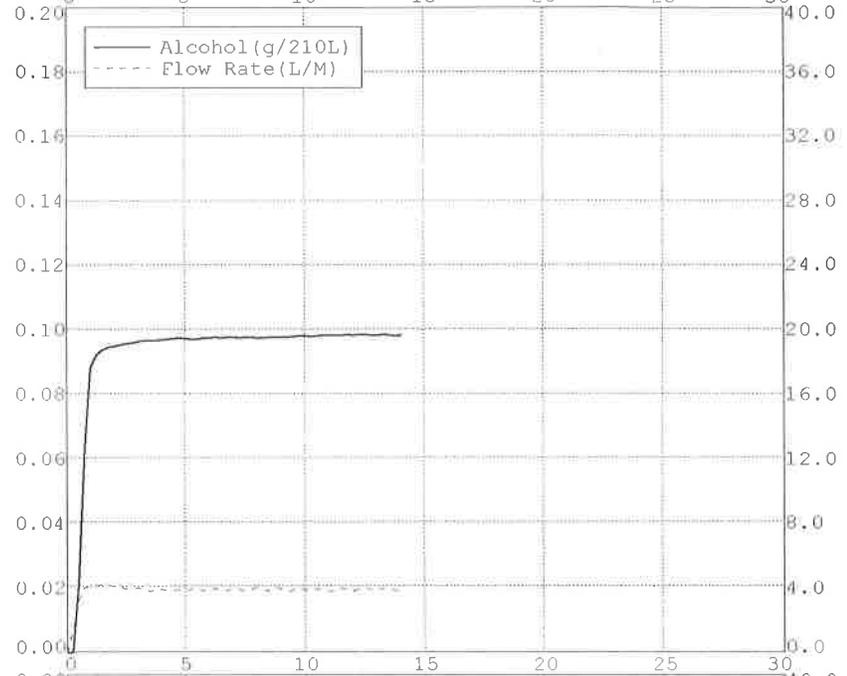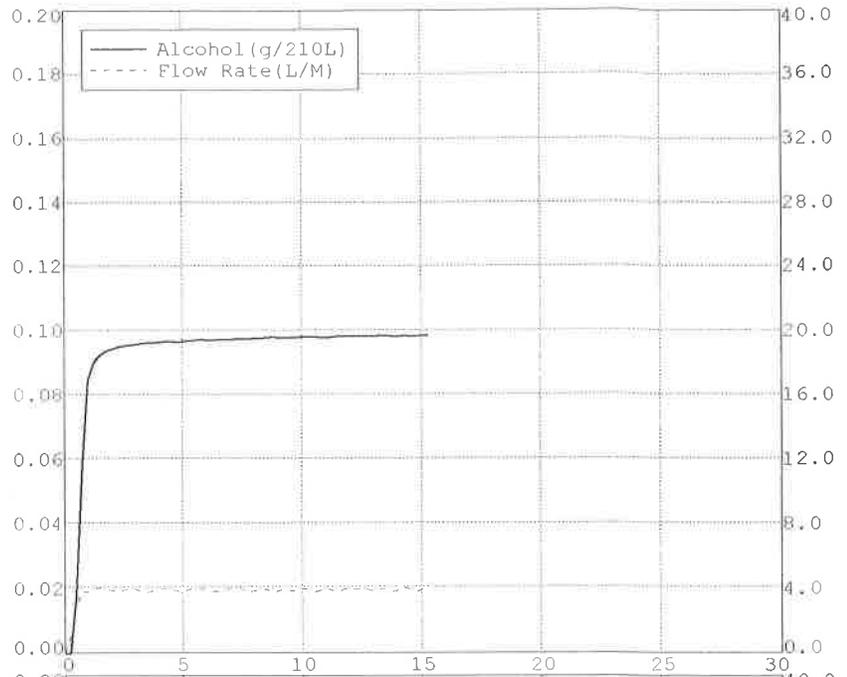

SUPERVISOR TEST

GLENS FALLS CITY
POLICE DEPT
DATAMASTER dmt: 117106

Date: 06/08/2020

OPERATOR NAME:
THOMAS S PRATT
Permit #: 48766
Operator Agency/Dept: GLENS FALLS CITY PD
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:46
INTERNAL STANDARD	VERIFIED	00:46
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	00:47
BLANK TEST	0.00	00:48
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	00:48
BLANK TEST	0.00	00:49
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	00:49

Blank Error

