

SUPERVISOR TEST




-----  
GLENS FALLS CITY  
POLICE DEPT  
DATAMASTER dmt: 117106  
-----

Date: 07/06/2020

OPERATOR NAME:  
THOMAS S PRATT  
Permit #: 48766  
Operator Agency/Dept: GLENS FALLS CITY PD  
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:24
INTERNAL STANDARD	VERIFIED	02:25
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	02:25
BLANK TEST	0.00	02:26
REFERENCE STANDARD TEMP	34.03c	
REFERENCE STANDARD	0.09	02:26
BLANK TEST	0.00	02:27
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	02:27
BLANK TEST	0.00	02:28

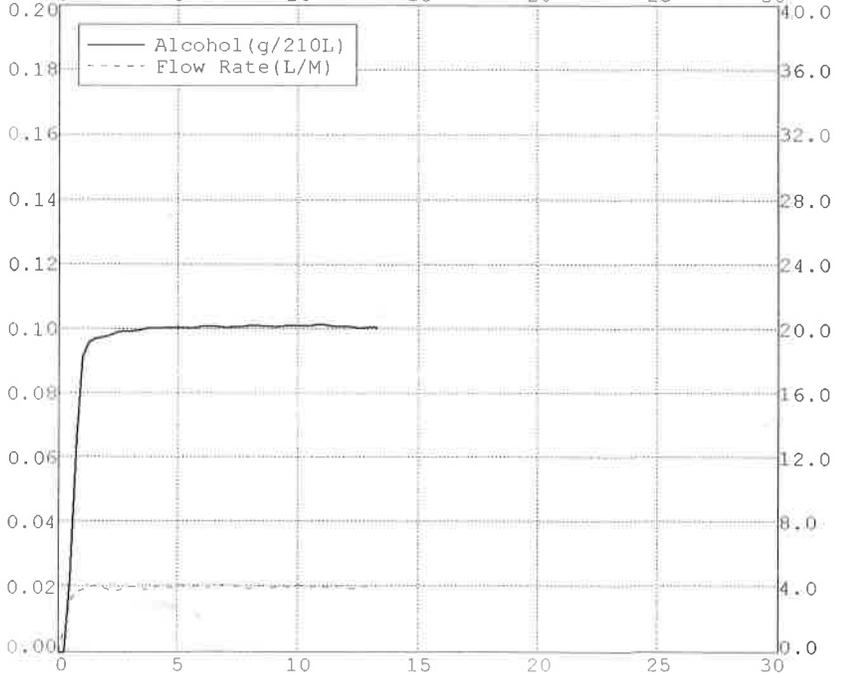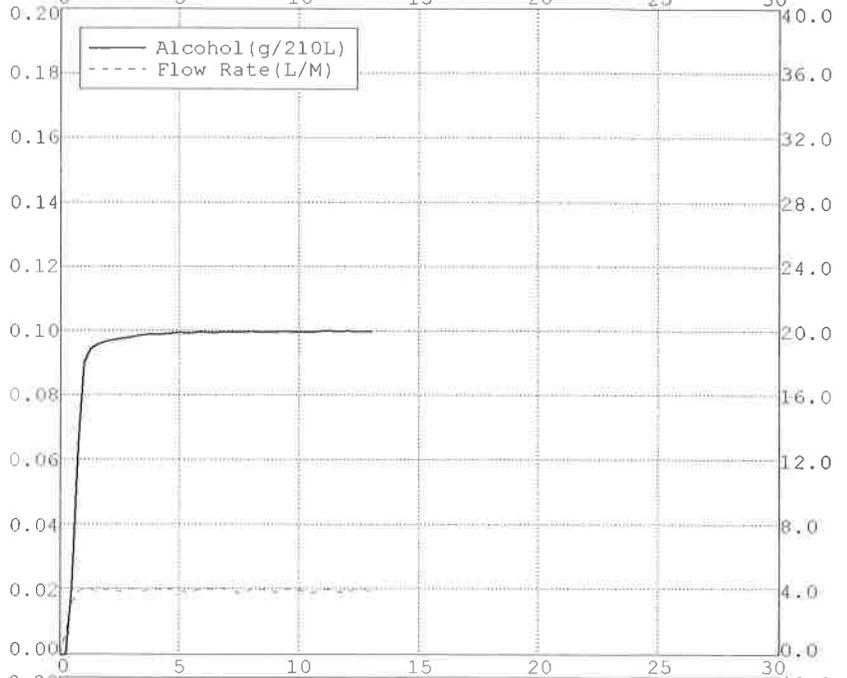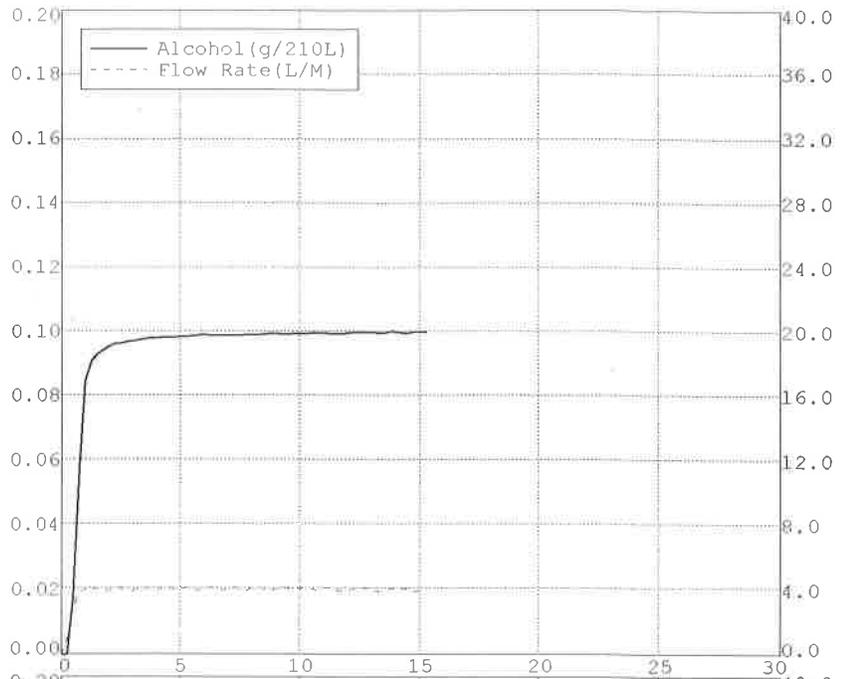

SUPERVISOR TEST

-----  
GLENS FALLS CITY  
POLICE DEPT  
DATAMASTER dmt: 117106  
-----




Date: 07/06/2020

OPERATOR NAME:  
THOMAS S PRATT  
Permit #: 48766  
Operator Agency/Dept: GLENS FALLS CITY PD  
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:14
INTERNAL STANDARD	VERIFIED	02:15
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	02:15
BLANK TEST	0.00	02:16
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	02:16
BLANK TEST	0.00	02:17
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	02:18

Blank Error

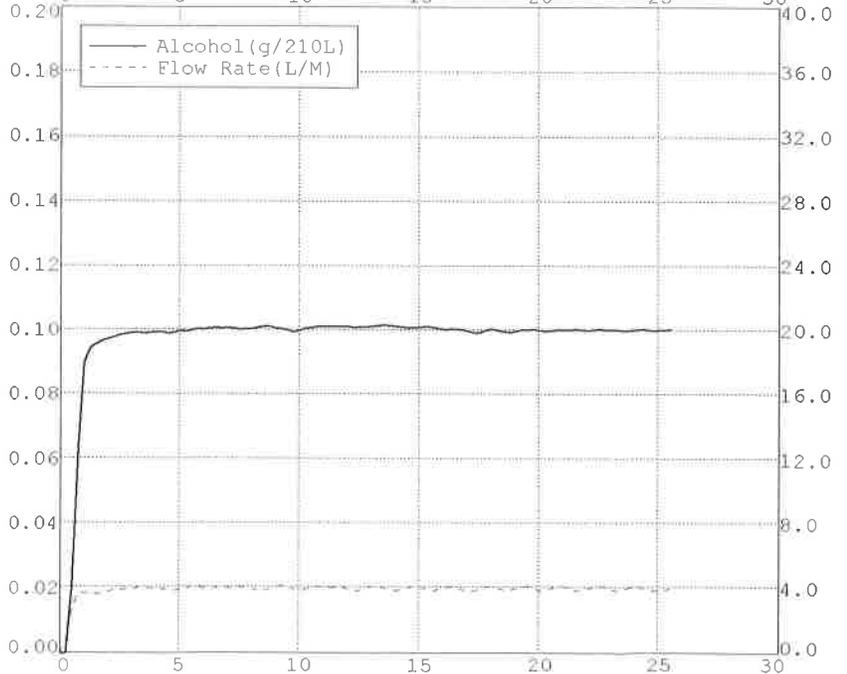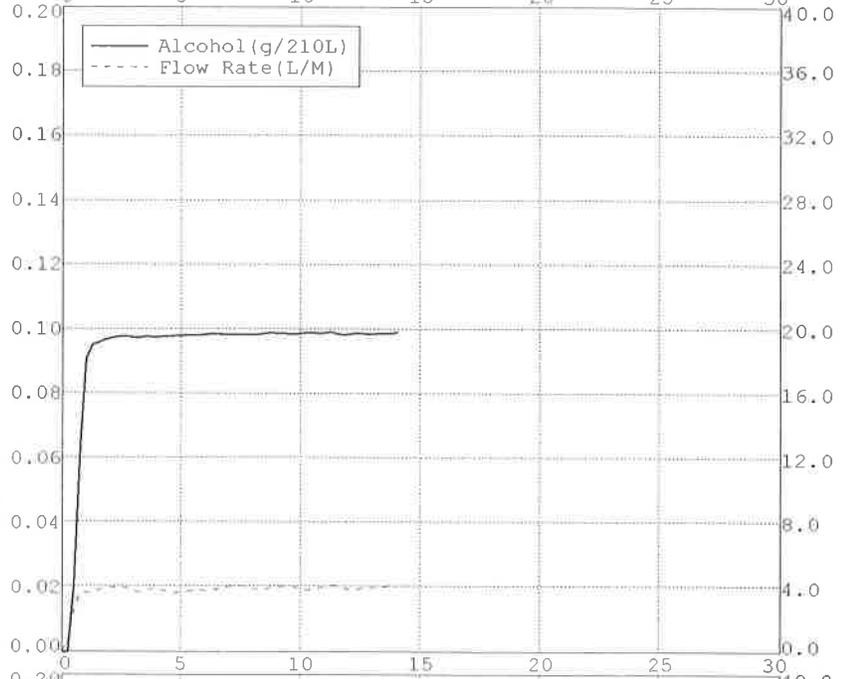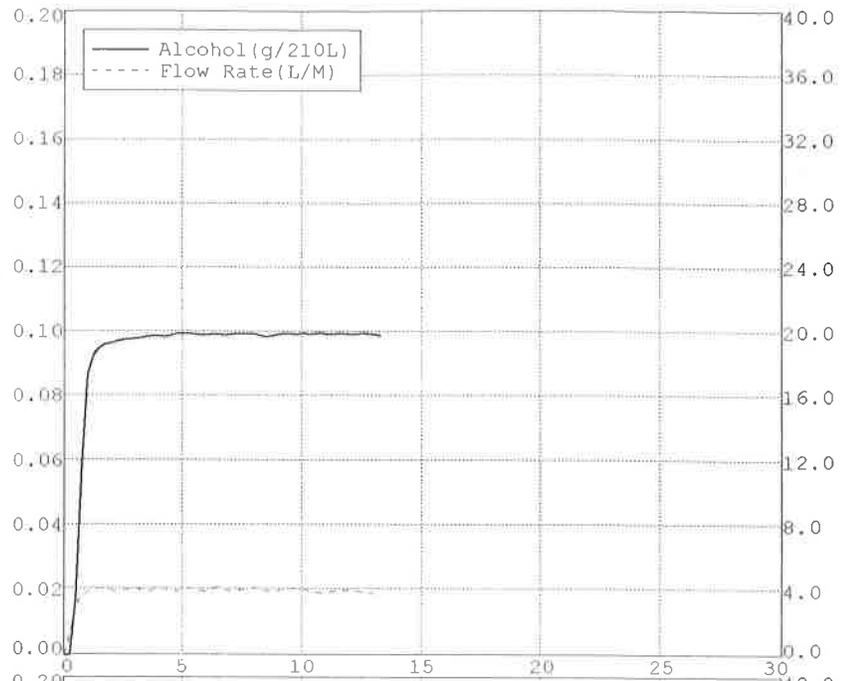

SUPERVISOR TEST

-----  
GLENS FALLS CITY  
POLICE DEPT  
DATAMASTER dmt: 117106  
-----



Date: 07/06/2020

OPERATOR NAME:  
THOMAS S PRATT  
Permit #: 48766  
Operator Agency/Dept: GLENS FALLS CITY PD  
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:01
INTERNAL STANDARD	VERIFIED	02:01
REFERENCE STANDARD TEMP	34.03c	
REFERENCE STANDARD	0.10	02:01
BLANK TEST	0.00	02:03
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	02:03

Blank Error

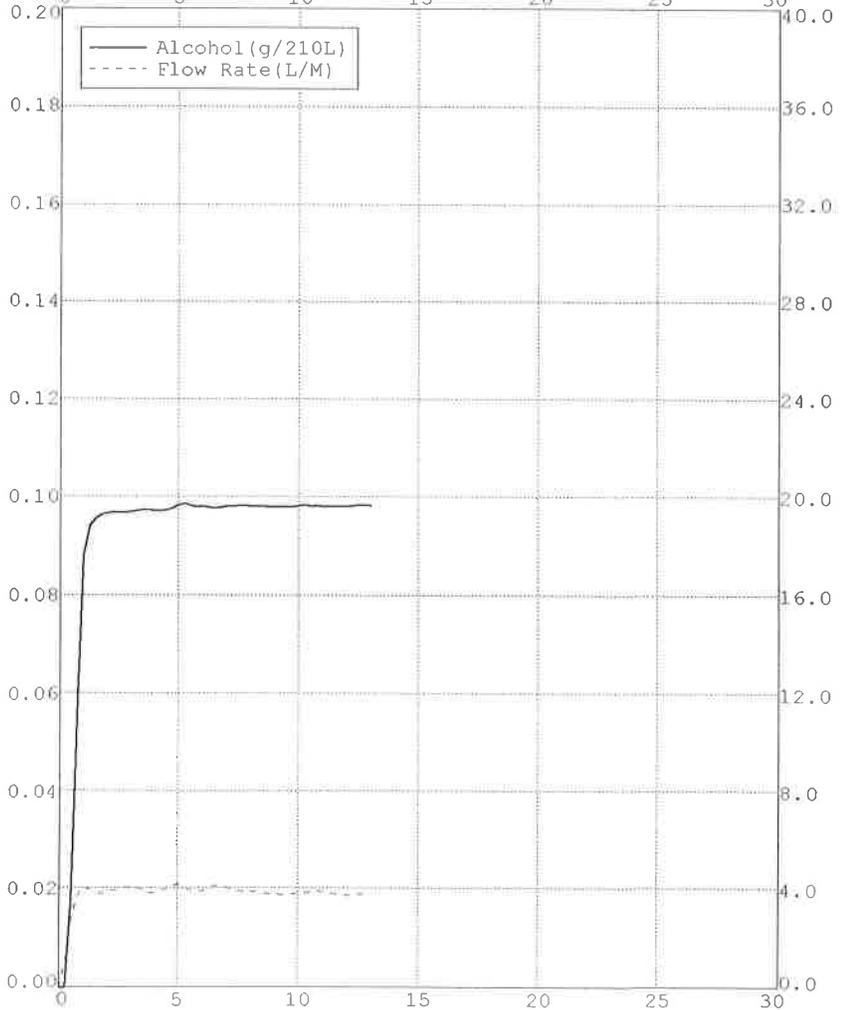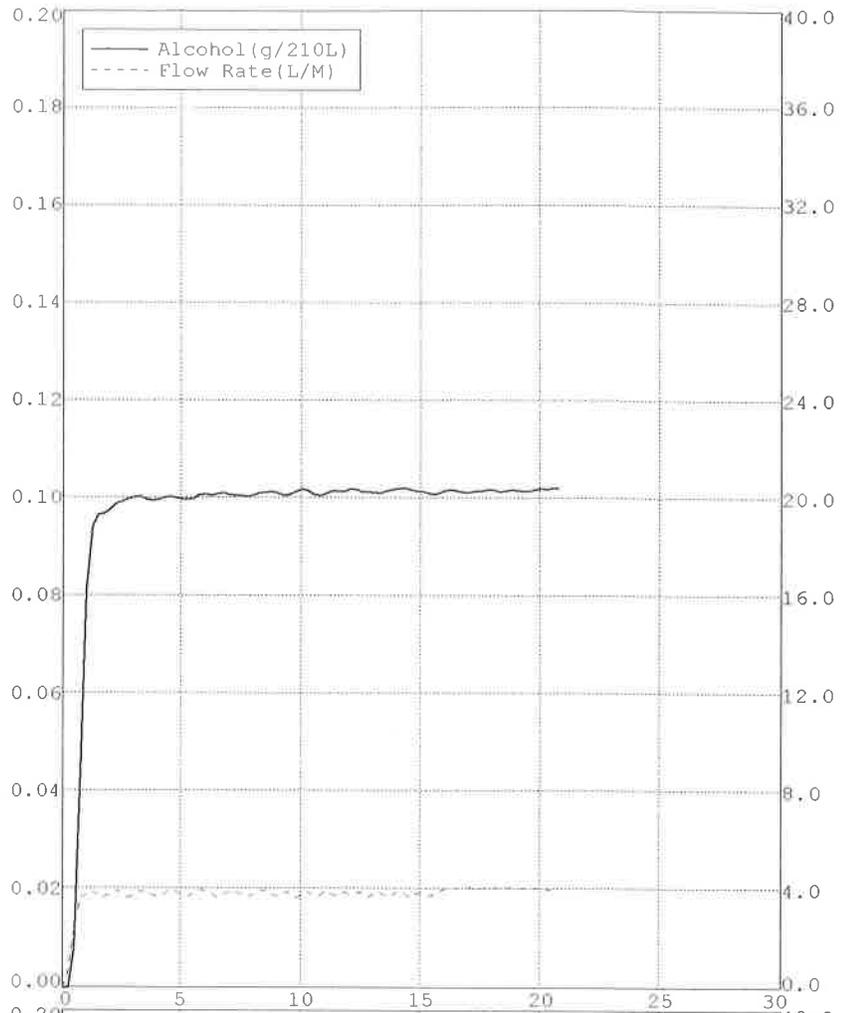

SUPERVISOR TEST

-----  
GLENS FALLS CITY  
POLICE DEPT  
DATAMASTER dmt: 117106  
-----

Date: 07/06/2020

OPERATOR NAME:  
THOMAS S PRATT  
Permit #: 48766  
Operator Agency/Dept: GLENS FALLS CITY PD  
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:09
INTERNAL STANDARD	VERIFIED	02:09
REFERENCE STANDARD TEMP	34.03c	
REFERENCE STANDARD	0.09	02:10

Blank Error

