

SUPERVISOR TEST




GLENS FALLS CITY
POLICE DEPT
DATAMASTER dmt: 117106

Date: 08/17/2020

OPERATOR NAME:
DESMOND L LYONS
Permit #: 35876
Operator Agency/Dept: GLENS FALLS CITY PD
Reference Standard #: 20240

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:43
INTERNAL STANDARD	VERIFIED	02:43
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	02:44
BLANK TEST	0.00	02:45
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	02:46
BLANK TEST	0.00	02:46
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	02:47
BLANK TEST	0.00	02:48

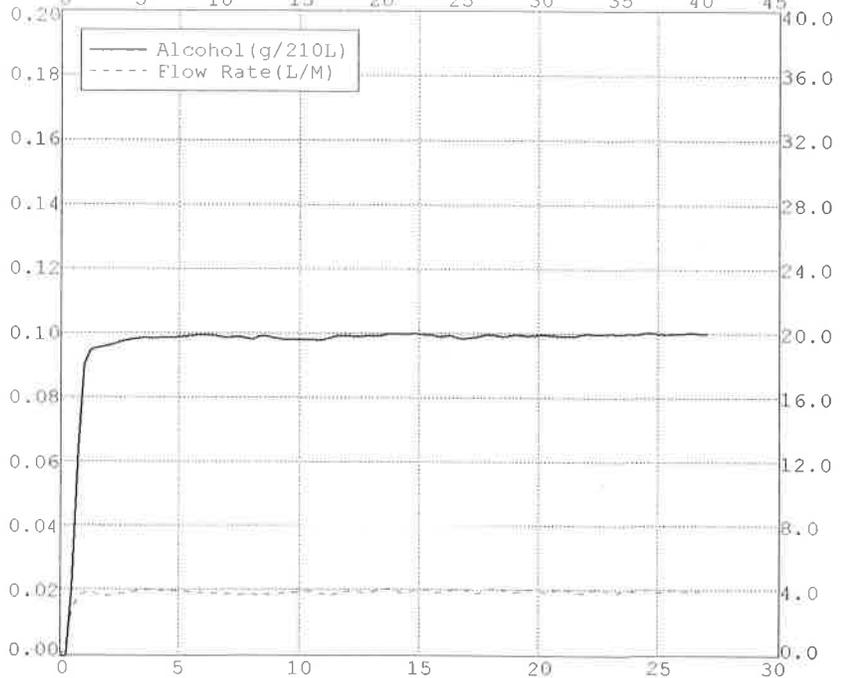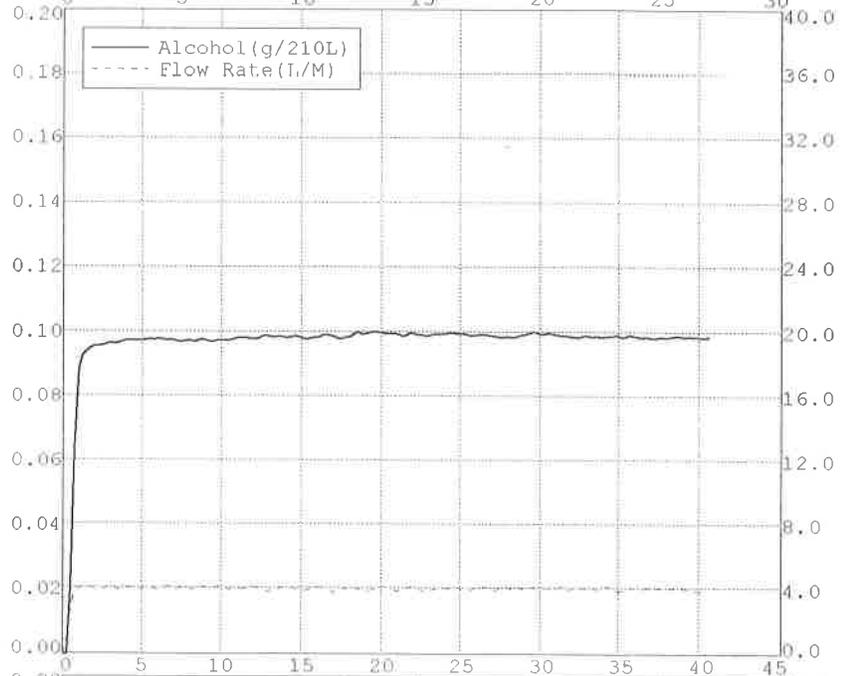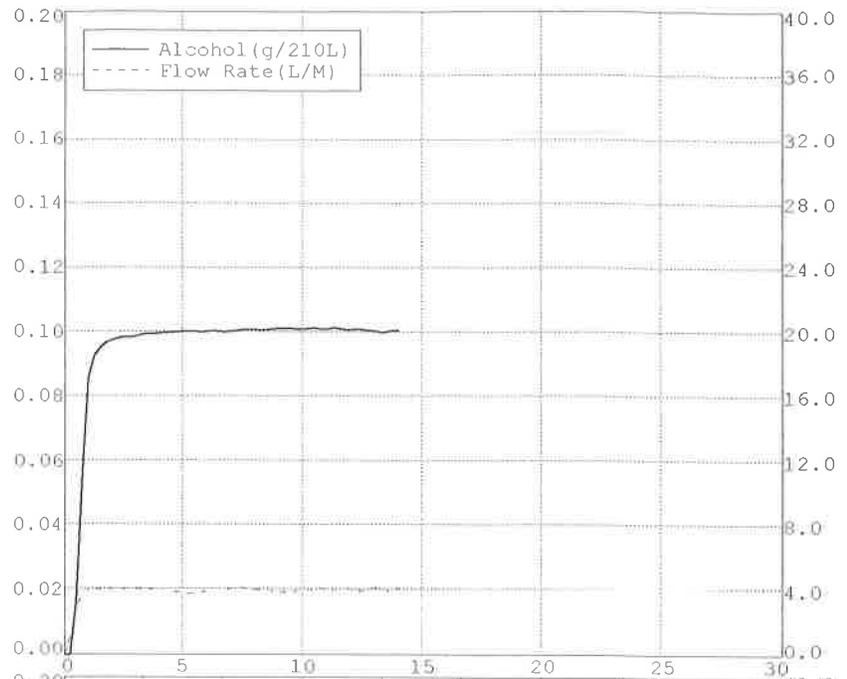

SUPERVISOR TEST

GLENS FALLS CITY
POLICE DEPT
DATAMASTER dmt: 117106

Date: 08/17/2020

OPERATOR NAME:
DESMOND L LYONS
Permit #: 35876
Operator Agency/Dept: GLENS FALLS CITY PD
Reference Standard #: 20240

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:39
INTERNAL STANDARD	VERIFIED	02:40

Simulator Timed Out