

SUPERVISOR TEST




-----  
GLENS FALLS CITY  
POLICE DEPT  
DATAMASTER dmt: 117106  
-----

Date: 08/31/2020

OPERATOR NAME:  
DESMOND L LYONS  
Permit #: 35876  
Operator Agency/Dept: GLENS FALLS CITY PD  
Reference Standard #: 20240

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:07
INTERNAL STANDARD	VERIFIED	23:07
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	23:08
BLANK TEST	0.00	23:09
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	23:09
BLANK TEST	0.00	23:10
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	23:10
BLANK TEST	0.00	23:11

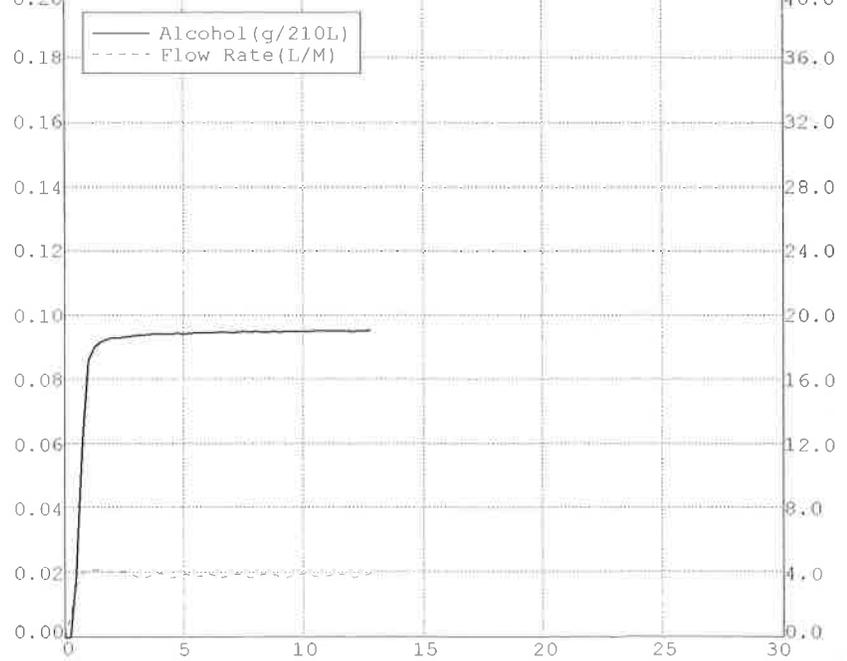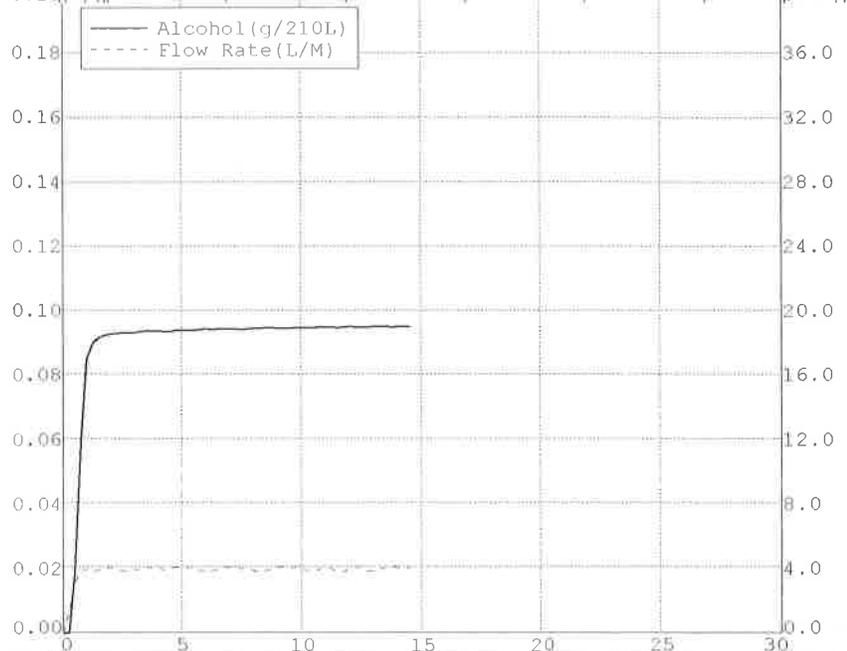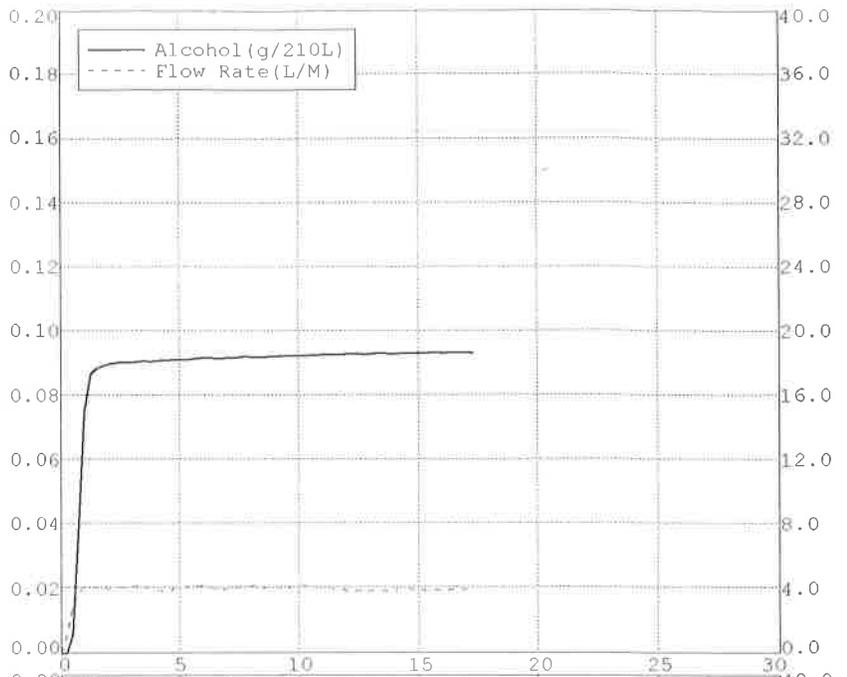

SOLUTION CHANGE

-----  
 GLENS FALLS CITY  
 POLICE DEPT  
 DATAMASTER dmt: 117106  
 -----

Date: 09/03/2020

OPERATOR NAME:  
 GERALD C WILLETTE  
 Permit #: 32550  
 Operator Agency/Dept: GLENS FALLS CITY PD  
 Reference Standard #: 20240

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:39
INTERNAL STANDARD	VERIFIED	03:40
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	03:40
BLANK TEST	0.00	03:41
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	03:41
BLANK TEST	0.00	03:42
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	03:42
BLANK TEST	0.00	03:43

