

SUPERVISOR TEST




GLENS FALLS CITY
POLICE DEPT
DATAMASTER dmt: 117106

Date: 09/28/2020

OPERATOR NAME:
NICHOLAS K RYSEDORPH
Permit #: 48769
Operator Agency/Dept: GLENS FALLS CITY PD
Reference Standard #: 20240

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 03:20 |
| INTERNAL STANDARD | VERIFIED | 03:20 |
| REFERENCE STANDARD TEMP | 34.02c | |
| REFERENCE STANDARD | 0.09 | 03:20 |
| BLANK TEST | 0.00 | 03:21 |
| REFERENCE STANDARD TEMP | 34.02c | |
| REFERENCE STANDARD | 0.09 | 03:21 |
| BLANK TEST | 0.00 | 03:22 |
| REFERENCE STANDARD TEMP | 34.02c | |
| REFERENCE STANDARD | 0.09 | 03:23 |
| BLANK TEST | 0.00 | 03:23 |

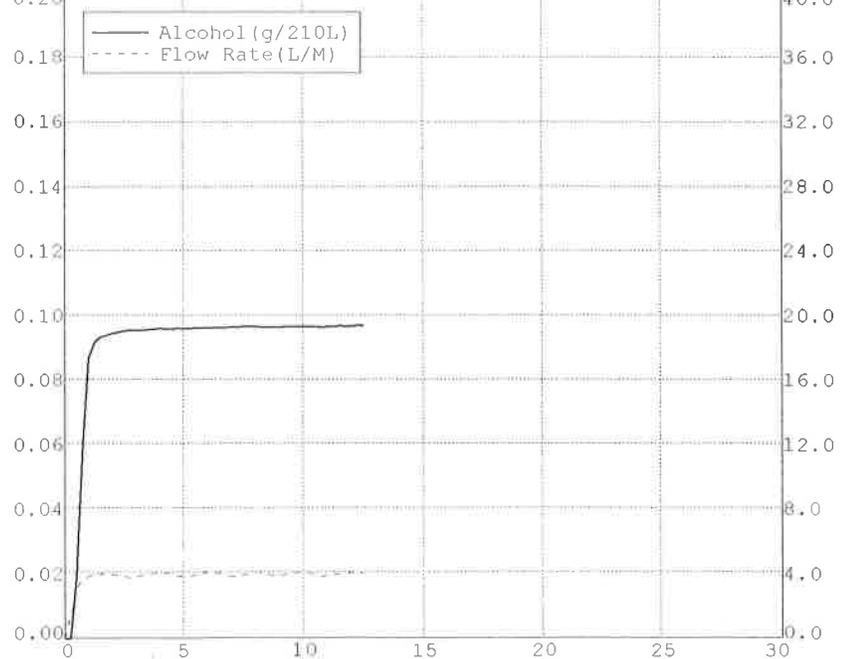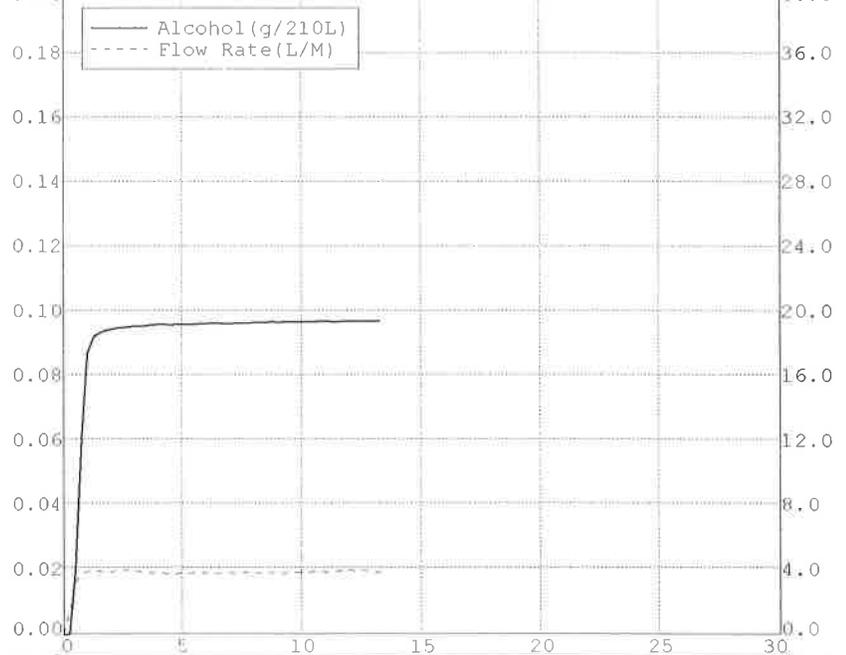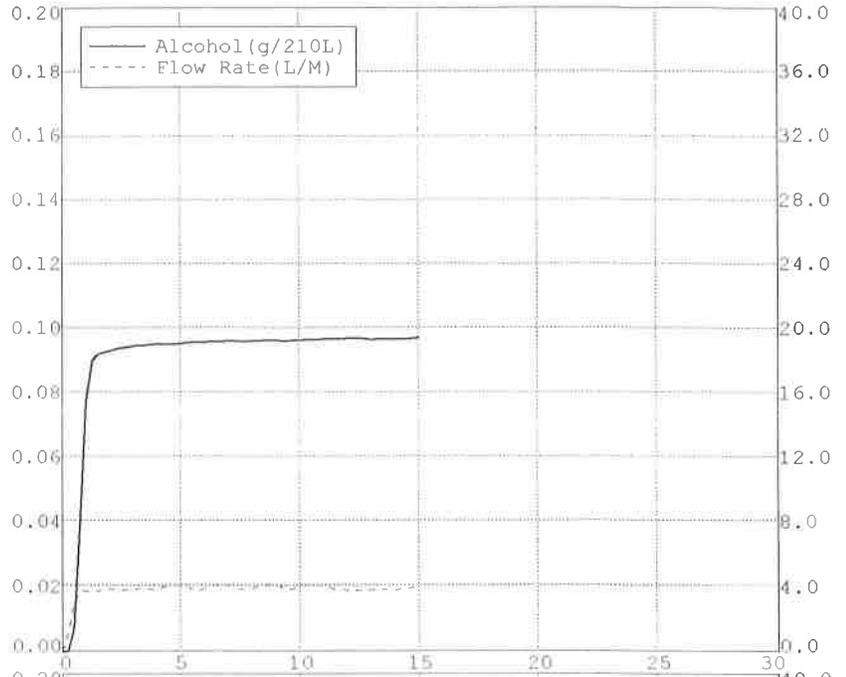

SOLUTION CHANGE




GLENS FALLS CITY
 POLICE DEPT
 DATAMASTER dmt: 117106

Date: 10/01/2020

OPERATOR NAME:
 DESMOND L LYONS
 Permit #: 35876
 Operator Agency/Dept: GLENS FALLS CITY PD
 Reference Standard #: 20340

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 02:04 |
| INTERNAL STANDARD | VERIFIED | 02:04 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 02:04 |
| BLANK TEST | 0.00 | 02:05 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 02:06 |
| BLANK TEST | 0.00 | 02:07 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 02:07 |
| BLANK TEST | 0.00 | 02:08 |

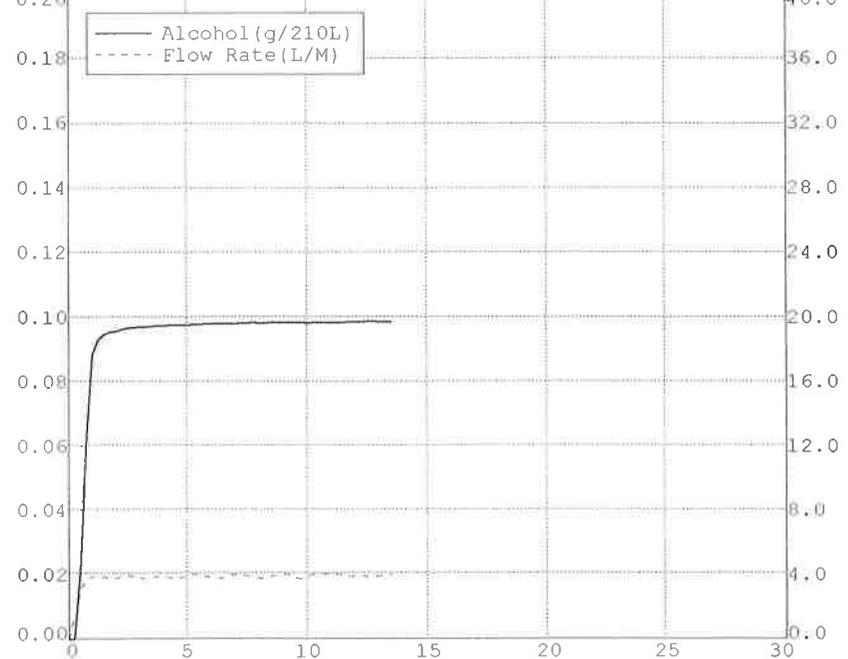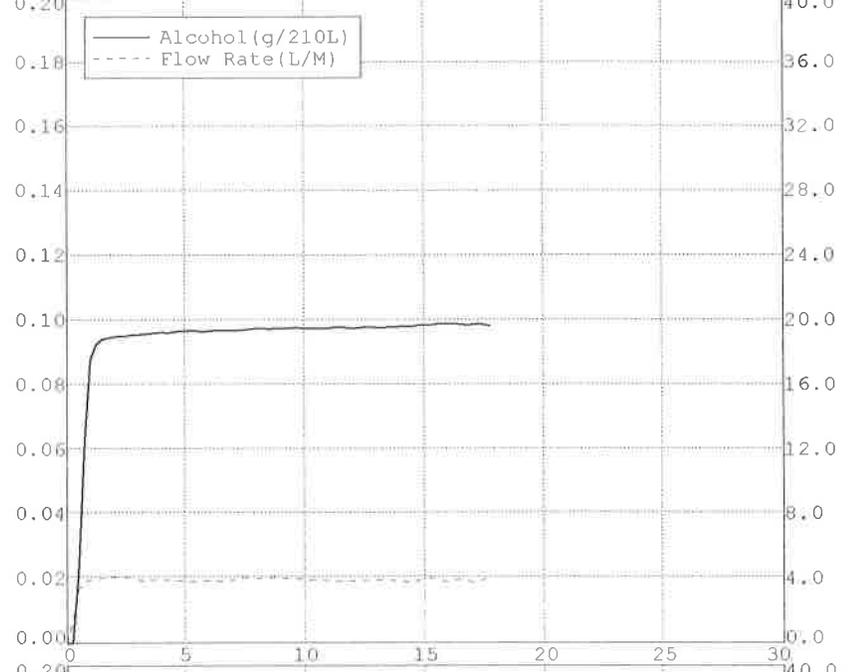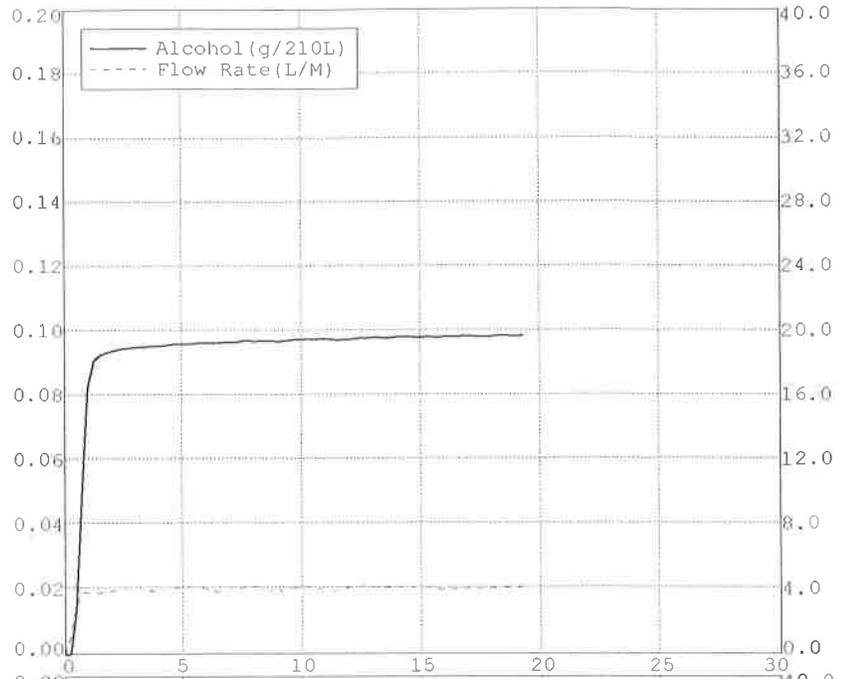

SUPERVISOR TEST



GLENS FALLS CITY
POLICE DEPT
DATAMASTER dmt: 117106

Date: 10/05/2020

OPERATOR NAME:
DESMOND L LYONS
Permit #: 35876
Operator Agency/Dept: GLENS FALLS CITY PD
Reference Standard #: 20340

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 02:53 |
| INTERNAL STANDARD | VERIFIED | 02:54 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 02:54 |
| BLANK TEST | 0.00 | 02:55 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 02:55 |
| BLANK TEST | 0.00 | 02:56 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 02:57 |
| BLANK TEST | 0.00 | 02:57 |

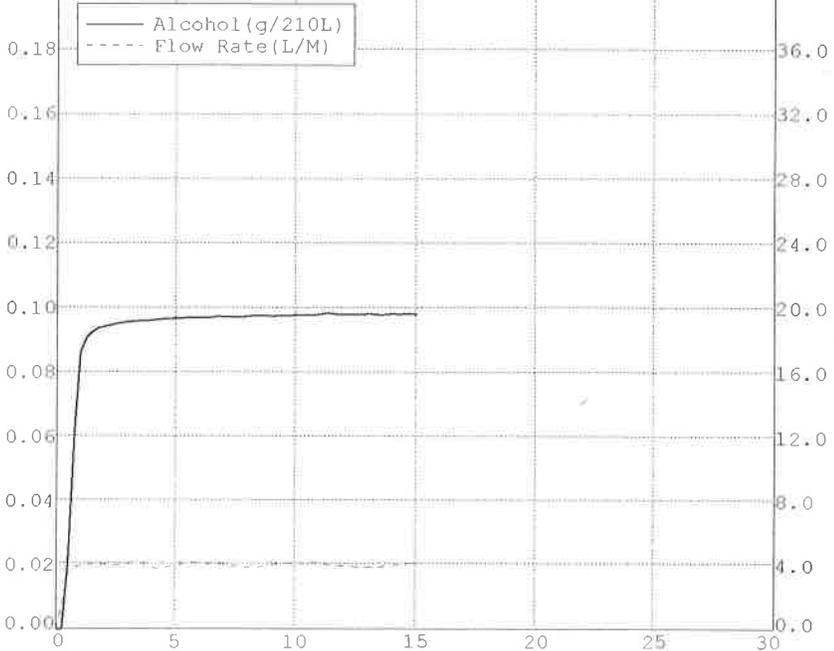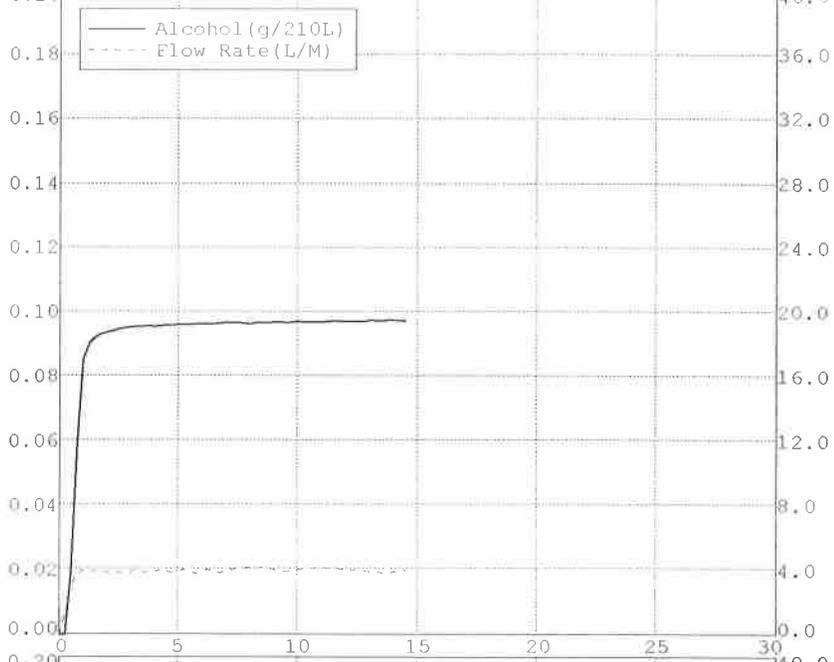

SUPERVISOR TEST

GLENS FALLS CITY
POLICE DEPT
DATAMASTER dmt: 117106

Date: 10/12/2020

OPERATOR NAME:
ROBERT M FOO
Permit #: 46059
Operator Agency/Dept: GLENS FALLS CITY PD
Reference Standard #: 20340

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 01:50 |
| INTERNAL STANDARD | VERIFIED | 01:51 |
| REFERENCE STANDARD TEMP | 34.02c | |
| REFERENCE STANDARD | 0.09 | 01:51 |
| BLANK TEST | 0.00 | 01:52 |
| REFERENCE STANDARD TEMP | 34.02c | |
| REFERENCE STANDARD | 0.09 | 01:52 |
| BLANK TEST | 0.00 | 01:53 |
| REFERENCE STANDARD TEMP | 34.02c | |
| REFERENCE STANDARD | 0.09 | 01:53 |
| BLANK TEST | 0.00 | 01:54 |

