

SUPERVISOR TEST




GLENS FALLS CITY
POLICE DEPT
DATAMASTER dmt: 117106

Date: 11/09/2020

OPERATOR NAME:
NICHOLAS K RYSEDORPH
Permit #: 48769
Operator Agency/Dept: GLENS FALLS CITY PD
Reference Standard #: 20340

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 00:49 |
| INTERNAL STANDARD | VERIFIED | 00:49 |
| REFERENCE STANDARD TEMP | 34.02c | |
| REFERENCE STANDARD | 0.09 | 00:49 |
| BLANK TEST | 0.00 | 00:50 |
| REFERENCE STANDARD TEMP | 34.02c | |
| REFERENCE STANDARD | 0.09 | 00:51 |
| BLANK TEST | 0.00 | 00:52 |
| REFERENCE STANDARD TEMP | 34.02c | |
| REFERENCE STANDARD | 0.09 | 00:52 |
| BLANK TEST | 0.00 | 00:53 |

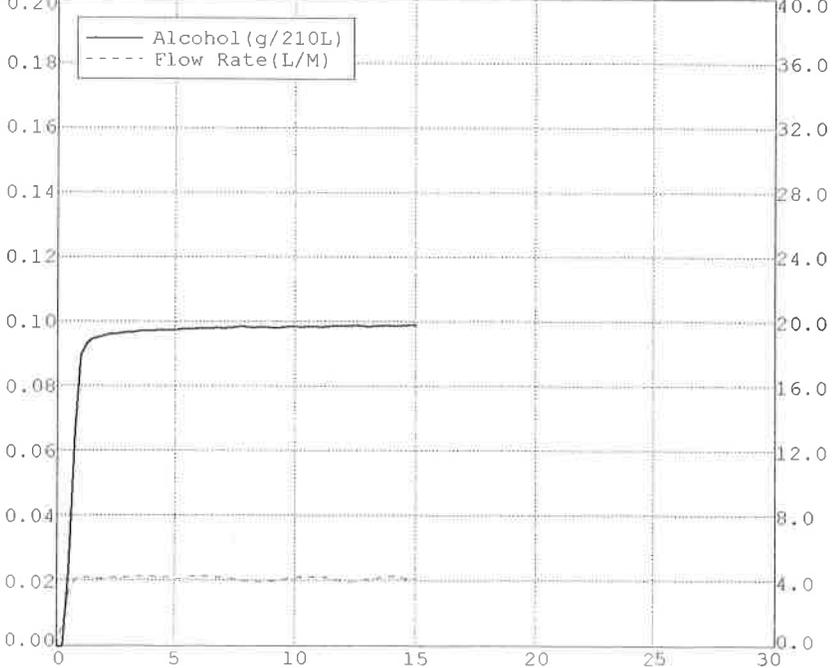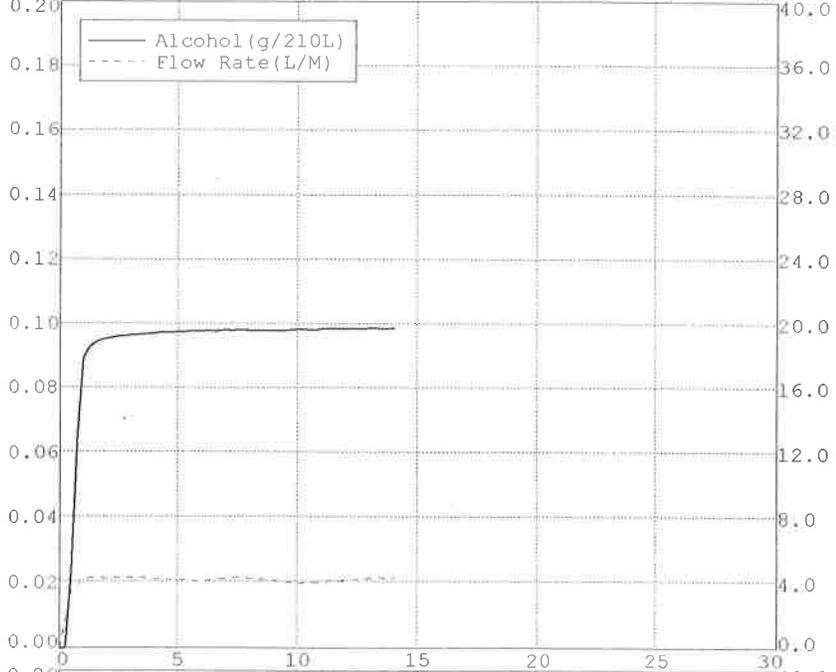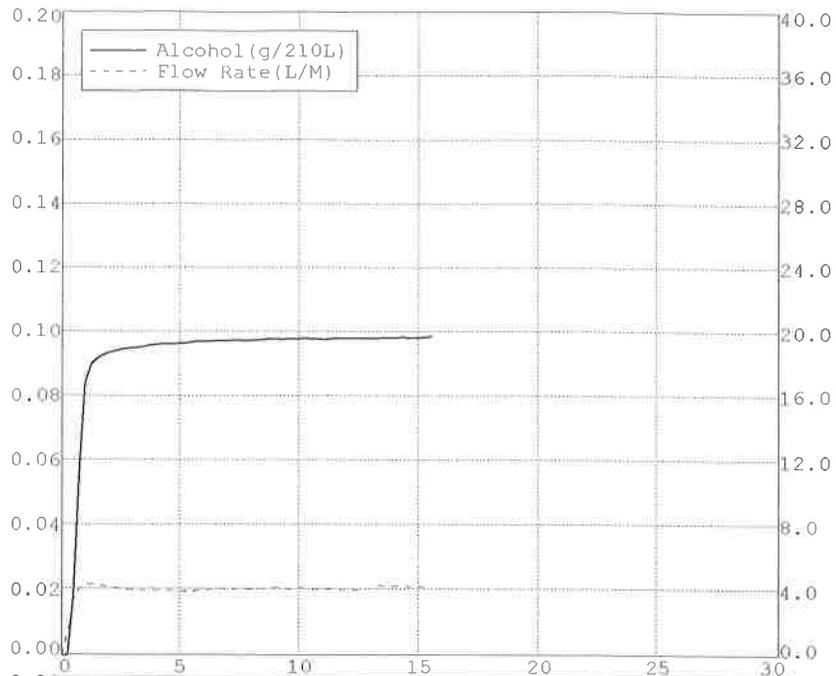

SUPERVISOR TEST

GLENS FALLS CITY
POLICE DEPT
DATAMASTER dmt: 117106

Date: 11/09/2020

OPERATOR NAME:
NICHOLAS K RYSEDORPH
Permit #: 48769
Operator Agency/Dept: GLENS FALLS CITY PD
Reference Standard #: 20340

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 00:40 |
| INTERNAL STANDARD | VERIFIED | 00:40 |
| REFERENCE STANDARD TEMP | 34.02c | |
| REFERENCE STANDARD | 0.09 | 00:41 |
| BLANK TEST | 0.00 | 00:42 |
| REFERENCE STANDARD TEMP | 34.02c | |
| REFERENCE STANDARD | 0.09 | 00:42 |

Blank Error

