

SUPERVISOR TEST



GLENS FALLS CITY
POLICE DEPT
DATAMASTER dmt: 117106

Date: 05/31/2021

OPERATOR NAME:
DESMOND L LYONS
Permit #: 35876
Operator Agency/Dept: GLENS FALLS CITY PD
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:47
INTERNAL STANDARD	VERIFIED	07:47
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	07:48
BLANK TEST	0.00	07:48
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	07:49
BLANK TEST	0.00	07:50
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	07:50
BLANK TEST	0.00	07:51

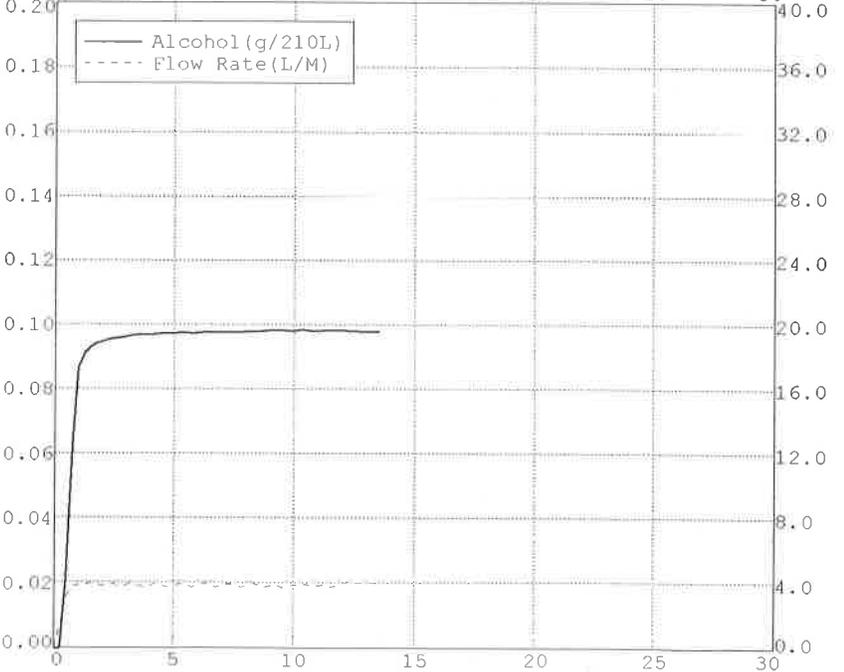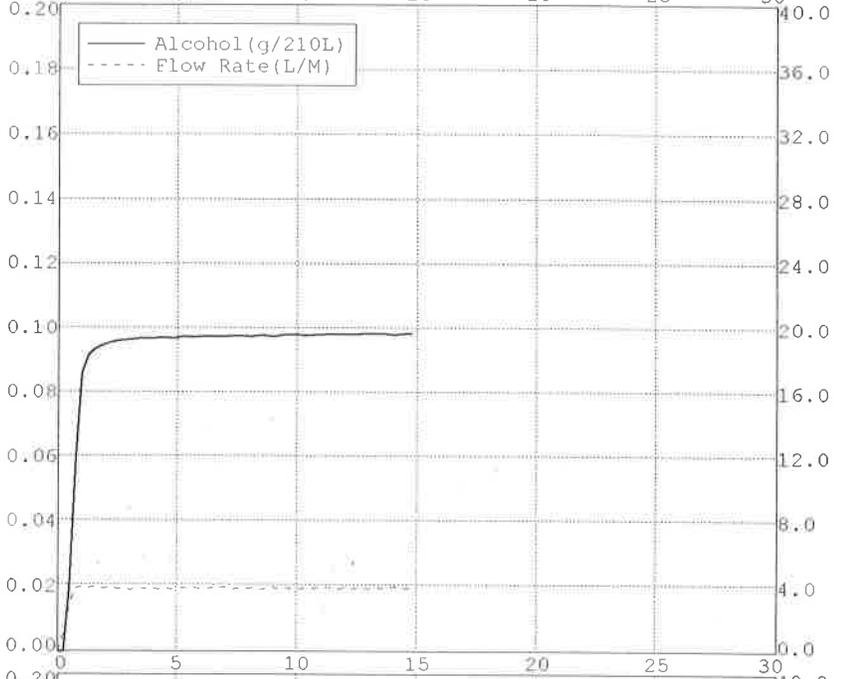

SOLUTION CHANGE




GLENS FALLS CITY
POLICE DEPT
DATAMASTER dmt: 117106

Date: 06/02/2021

OPERATOR NAME:
SHAWN A LOVELACE
Permit #: 30657
Operator Agency/Dept: GLENS FALLS CITY PD
Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:34
INTERNAL STANDARD	VERIFIED	00:35
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	00:35
BLANK TEST	0.00	00:36
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	00:36
BLANK TEST	0.00	00:37
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	00:37
BLANK TEST	0.00	00:38

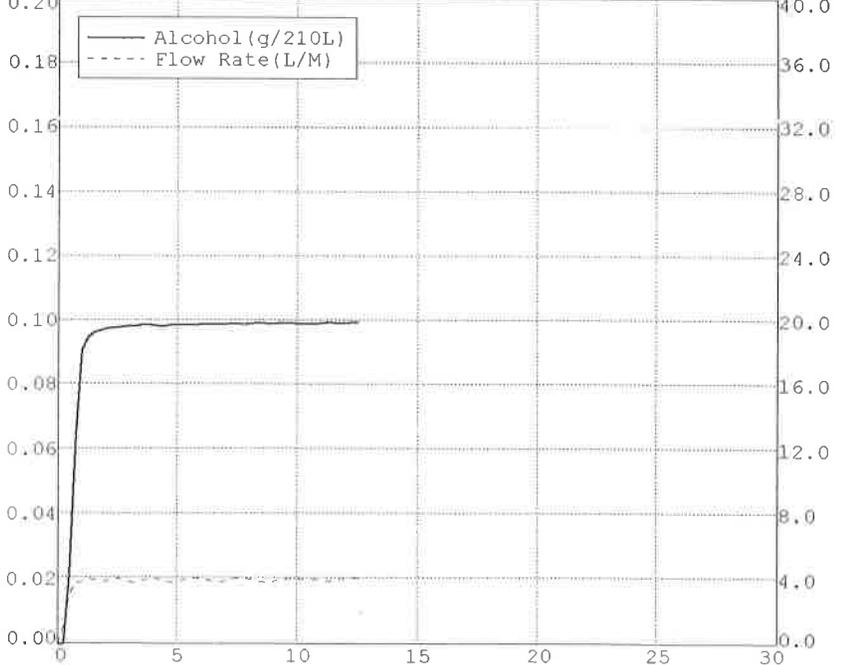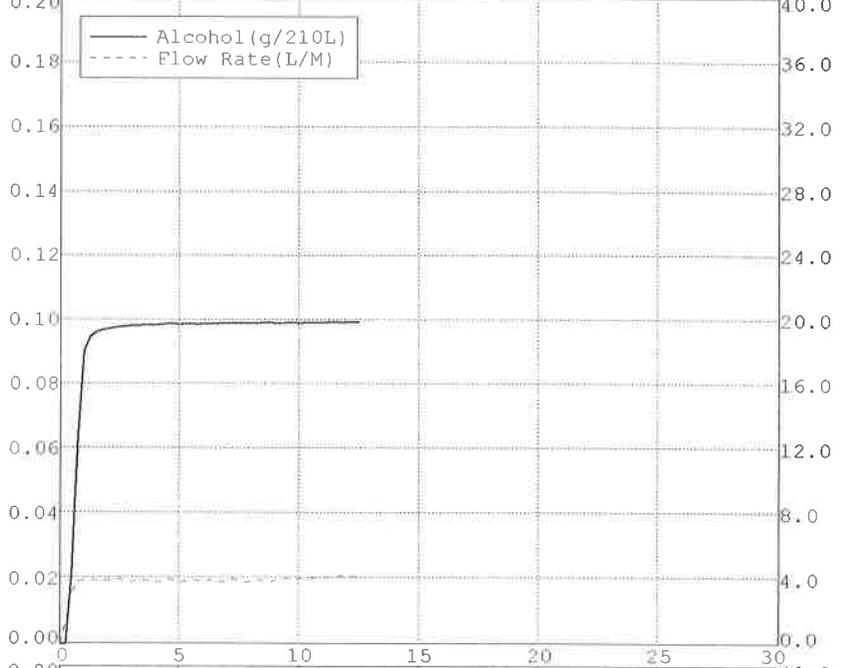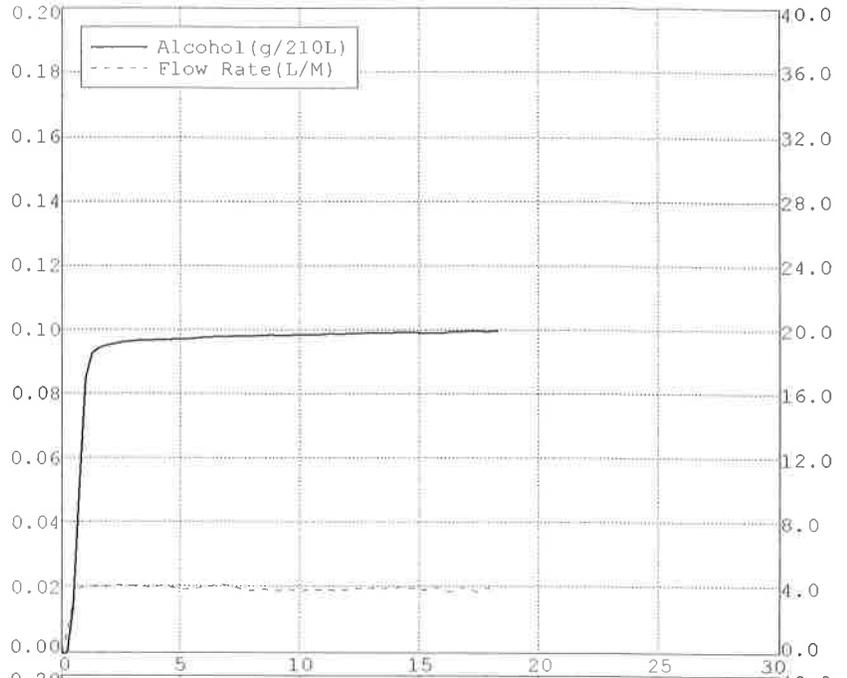

OW

SUPERVISOR TEST



GLENS FALLS CITY
POLICE DEPT
DATAMASTER dmt: 117106

Date: 06/07/2021

OPERATOR NAME:
JOHN F HOGAN
Permit #: 49269
Operator Agency/Dept: GLENS FALLS CITY PD
Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:54
INTERNAL STANDARD	VERIFIED	01:54
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	01:55
BLANK TEST	0.00	01:56
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	01:56
BLANK TEST	0.00	01:57
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	01:57
BLANK TEST	0.00	01:58

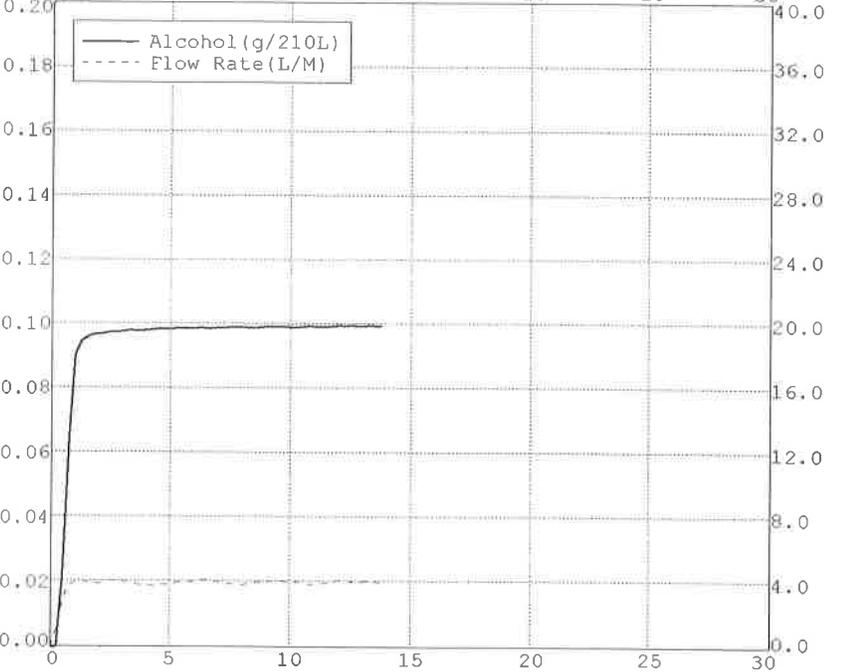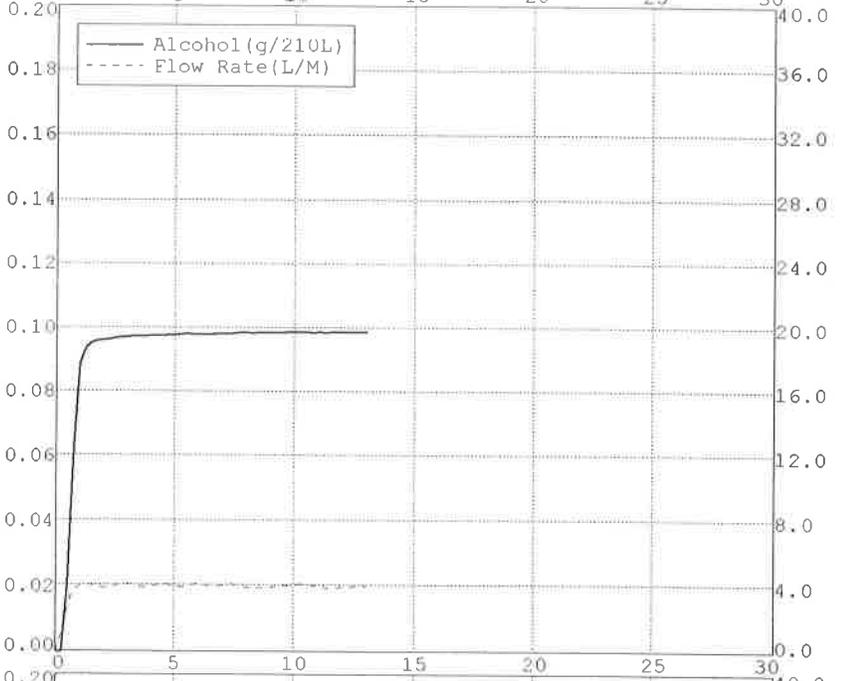



**Department
of Health**

Wadsworth
Center

This Permit Certifies That

FOO, ROBERT M.

Permit Number 46059

is a Breath Analysis Operator Certified in

NPAS DATAMASTER DMT from 07/28/2021 to 07/28/2023

Continuously certified in Breath Alcohol Instrumentation
since 7/28/2017
