

SUPERVISOR TEST




-----  
GLENS FALLS CITY  
POLICE DEPT  
DATAMASTER dmt: 117106  
-----

Date: 08/30/2021

OPERATOR NAME:  
SHAWN A LOVELACE  
Permit #: 30657  
Operator Agency/Dept: GLENS FALLS CITY PD  
Reference Standard #: 21170

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:20
INTERNAL STANDARD	VERIFIED	09:20
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	09:20
BLANK TEST	0.00	09:21
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	09:21
BLANK TEST	0.00	09:22
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	09:22
BLANK TEST	0.00	09:23

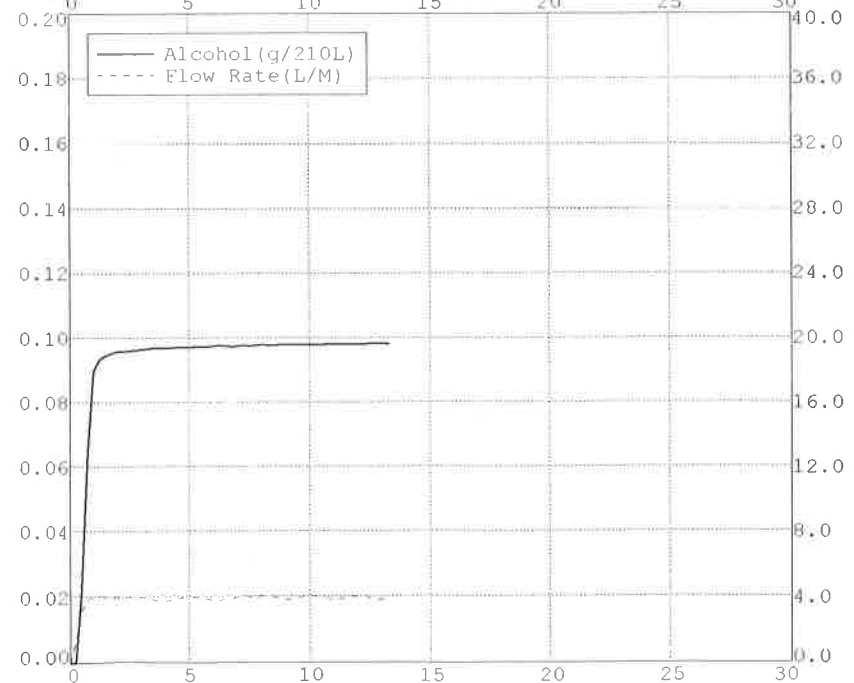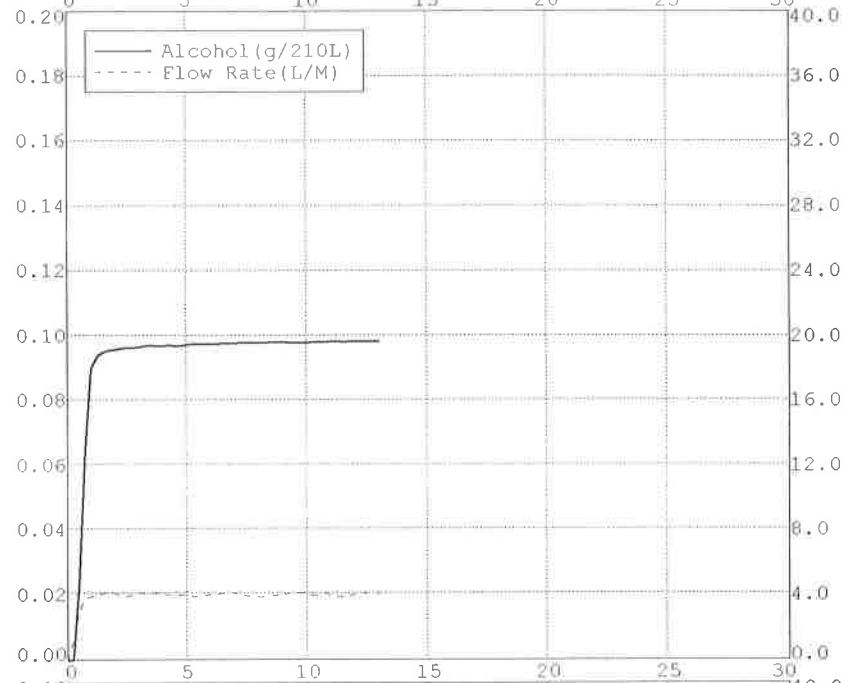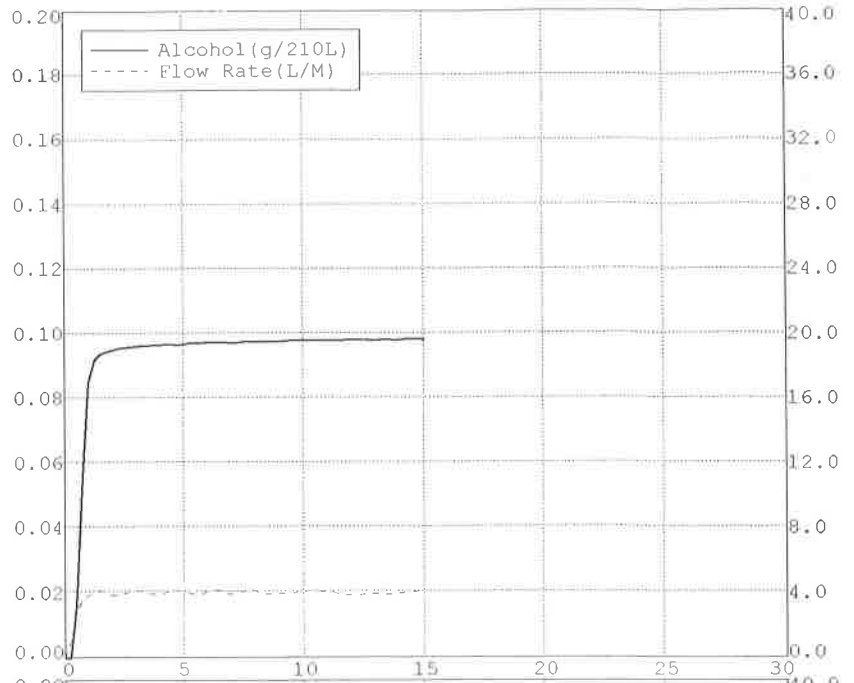

SOLUTION CHANGE

-----  
 GLENS FALLS CITY  
 POLICE DEPT  
 DATAMASTER dmt: 117106  
 -----

Date: 09/01/2021

OPERATOR NAME:  
 CARL P MATISON  
 Permit #: 42435  
 Operator Agency/Dept: GLENS FALLS CITY PD  
 Reference Standard #: 21170

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:19
INTERNAL STANDARD	VERIFIED	08:19
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	08:20
BLANK TEST	0.00	08:21
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	08:21
BLANK TEST	0.00	08:22
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	08:22
BLANK TEST	0.00	08:23

