

SUPERVISOR TEST



GLENS FALLS CITY
POLICE DEPT
DATAMASTER dmt: 117106

Date: 10/11/2021

OPERATOR NAME:
CRAIG M RAGGI
Permit #: 49219
Operator Agency/Dept: GLENS FALLS CITY PD
Reference Standard #: 21280

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:57
INTERNAL STANDARD	VERIFIED	02:57
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	02:57
BLANK TEST	0.00	02:58
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	02:59
BLANK TEST	0.00	02:59
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	03:00
BLANK TEST	0.00	03:01

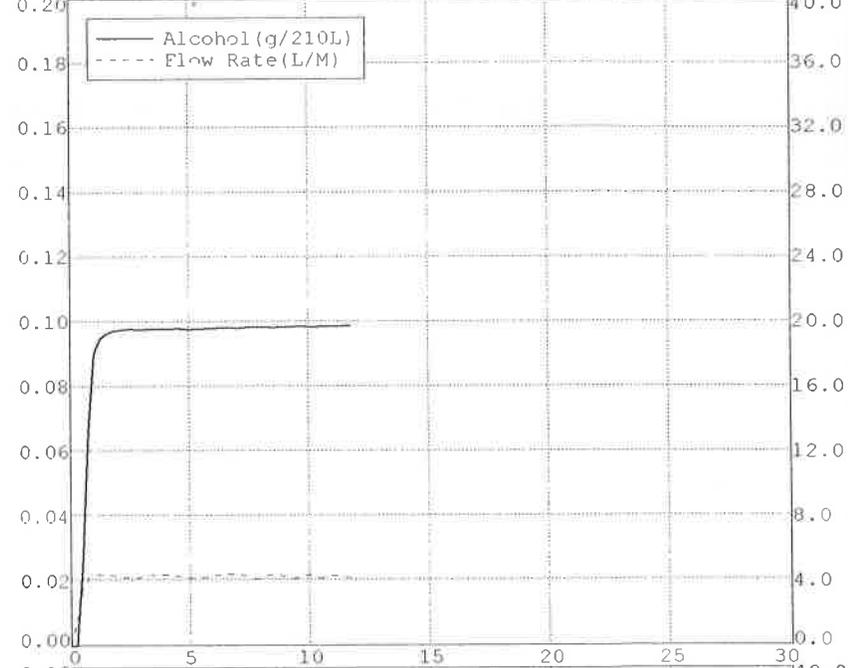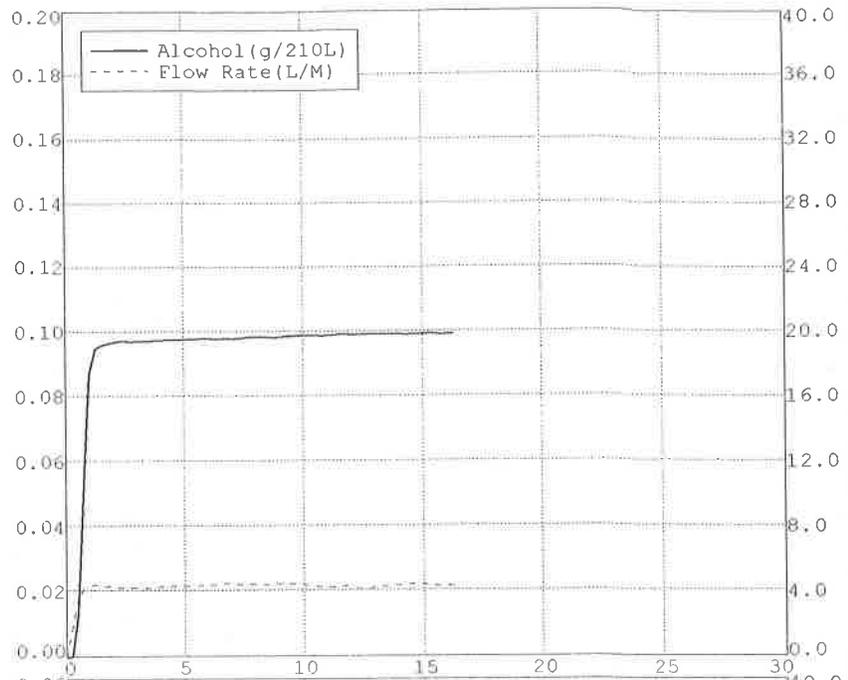

SOLUTION CHANGE

GLENS FALLS CITY
POLICE DEPT
DATAMASTER dmt: 117106

Date: 10/04/2021

OPERATOR NAME:
TYLER R MELLO
Permit #: 46781
Operator Agency/Dept: GLENS FALLS CITY PD
Reference Standard #: 21280

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:32
INTERNAL STANDARD	VERIFIED	00:32
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	00:33
BLANK TEST	0.00	00:34
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	00:34
BLANK TEST	0.00	00:35
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	00:35
BLANK TEST	0.00	00:36

