

SUPERVISOR TEST




GLENS FALLS CITY
POLICE DEPT
DATAMASTER dmt: 117106

Date: 11/15/2021

OPERATOR NAME:
CRAIG M RAGGI
Permit #: 49219
Operator Agency/Dept: GLENS FALLS CITY PD
Reference Standard #: 21280

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:11
INTERNAL STANDARD	VERIFIED	02:11
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	02:12
BLANK TEST	0.00	02:13
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	02:13
BLANK TEST	0.00	02:14
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	02:14
BLANK TEST	0.00	02:15

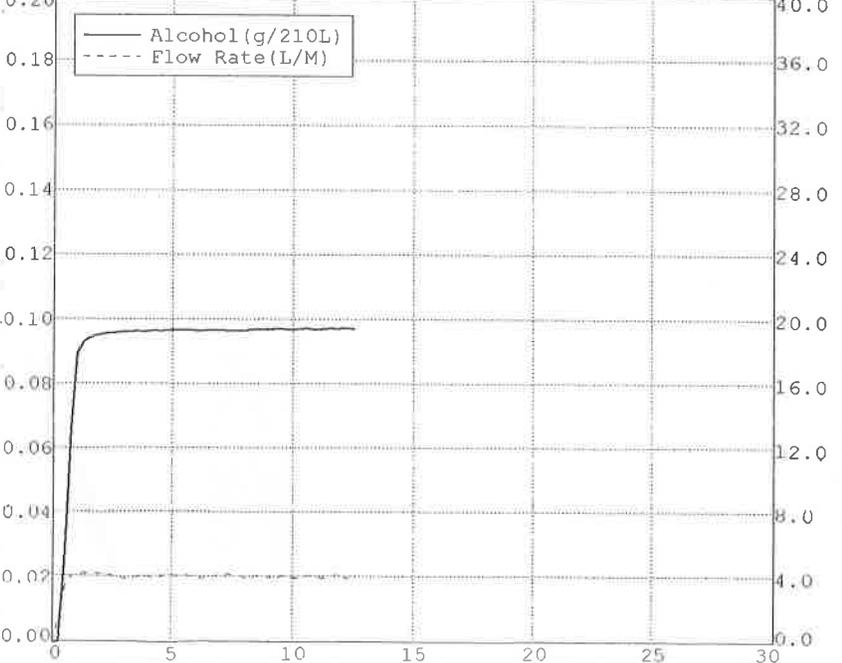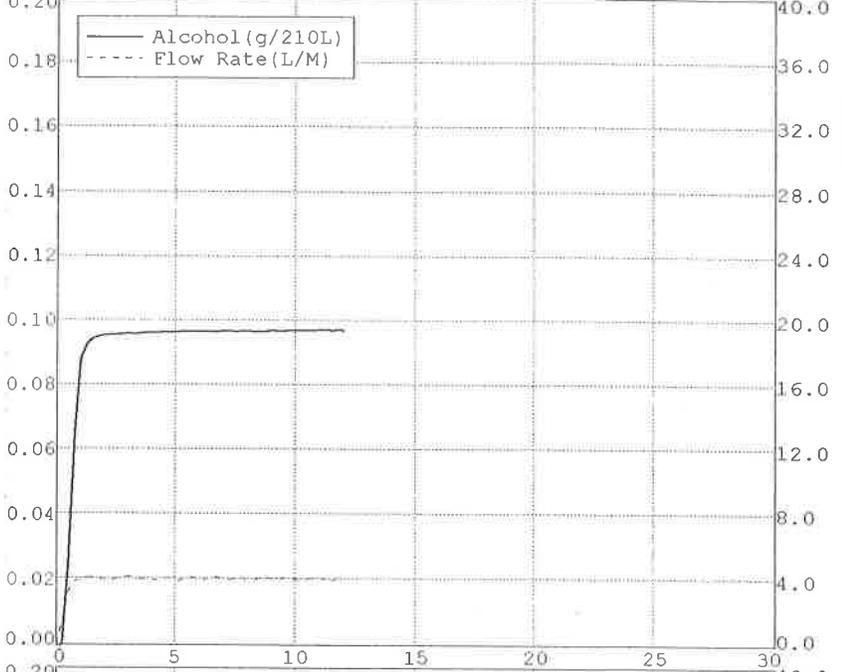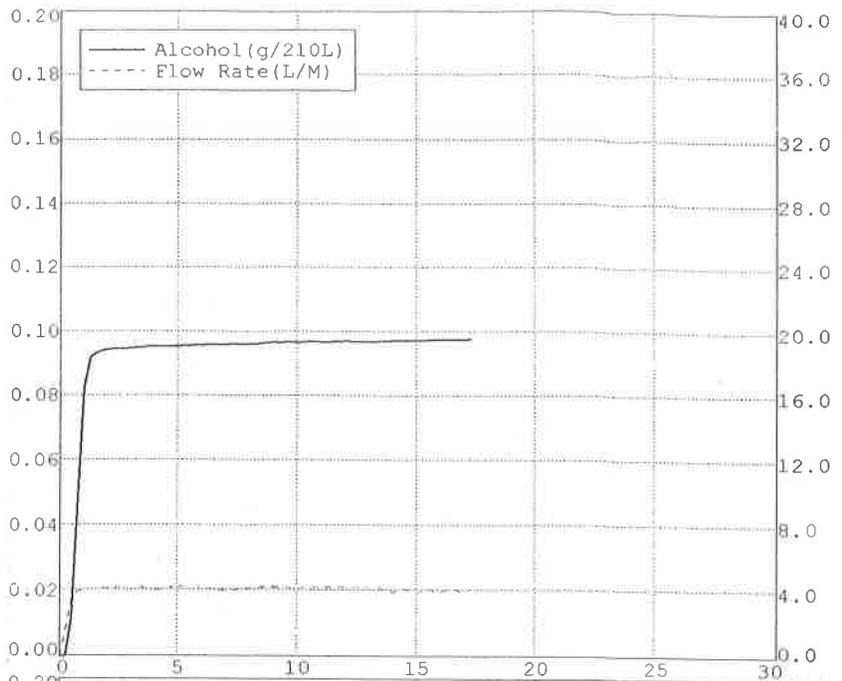

SUPERVISOR TEST

GLENS FALLS CITY
POLICE DEPT
DATAMASTER dmt: 117106

Date: 11/22/2021

OPERATOR NAME:
KEITH D SEEBODE
Permit #: 45900
Operator Agency/Dept: GLENS FALLS CITY PD
Reference Standard #: 21280

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:30
INTERNAL STANDARD	VERIFIED	01:30
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	01:30
BLANK TEST	0.00	01:31
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	01:31
BLANK TEST	0.00	01:32
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	01:32
BLANK TEST	0.00	01:33

