

SUPERVISOR TEST



GLENS FALLS CITY
POLICE DEPT
DATAMASTER dmt: 117106

Date: 01/03/2022

OPERATOR NAME:
CRAIG M RAGGI
Permit #: 49219
Operator Agency/Dept: GLENS FALLS CITY PD
Reference Standard #: 21390

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:21
INTERNAL STANDARD	VERIFIED	00:21
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	00:21
BLANK TEST	0.00	00:22
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	00:22
BLANK TEST	0.00	00:23
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	00:24
BLANK TEST	0.00	00:25

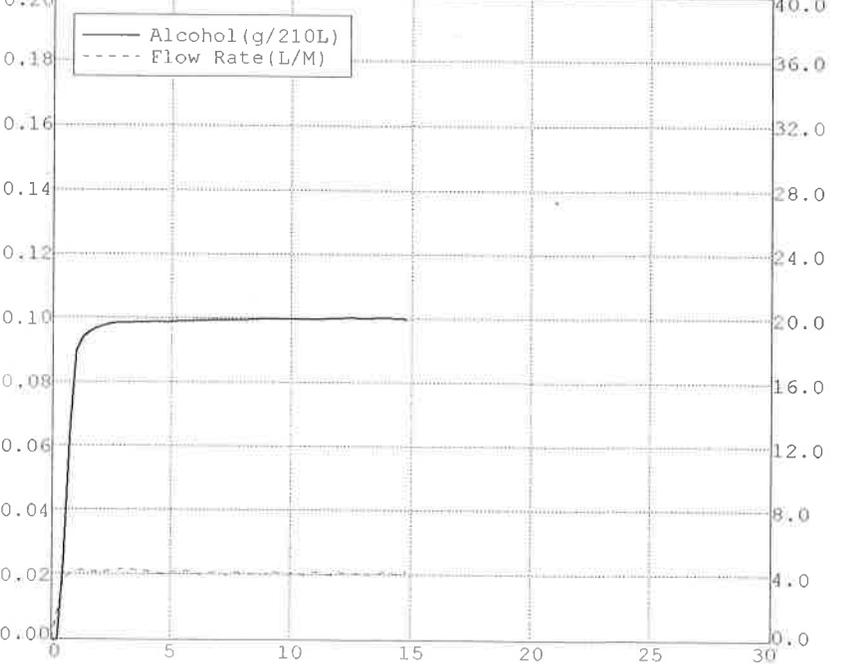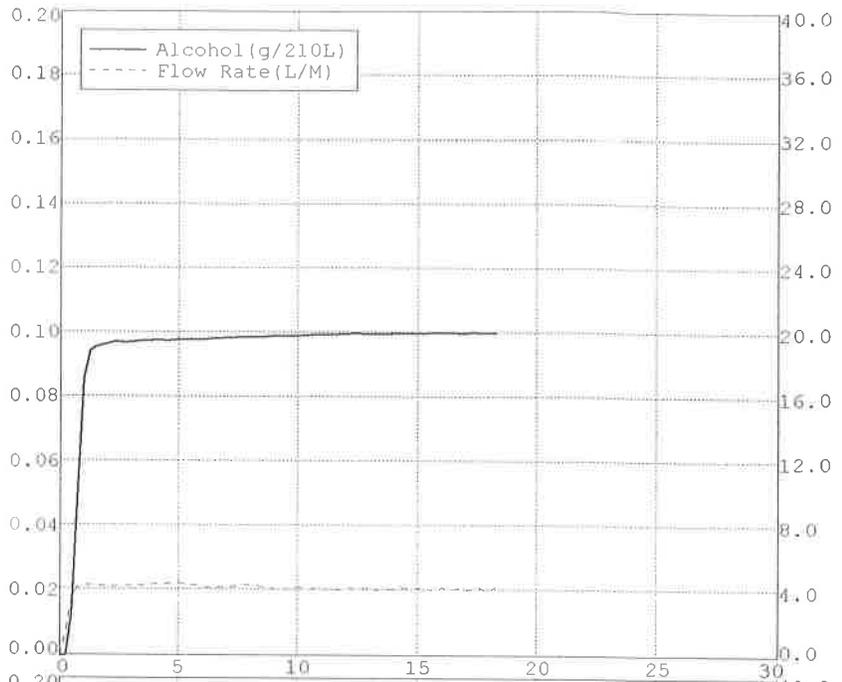

SOLUTION CHANGE

GLENS FALLS CITY
POLICE DEPT
DATAMASTER dmt: 117106

Date: 01/01/2022

OPERATOR NAME:
RYAN S PEDONE
Permit #: 35878
Operator Agency/Dept: GLENS FALLS CITY PD
Reference Standard #: 21390

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:10
INTERNAL STANDARD	VERIFIED	06:10
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	06:10
BLANK TEST	0.00	06:11
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	06:11
BLANK TEST	0.00	06:12
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	06:13
BLANK TEST	0.00	06:14

