

SUPERVISOR TEST




GLENS FALLS CITY
POLICE DEPT
DATAMASTER dmt: 117106

Date: 01/31/2022

OPERATOR NAME:
CRAIG M RAGGI
Permit #: 49219
Operator Agency/Dept: GLENS FALLS CITY PD
Reference Standard #: 21390

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:40
INTERNAL STANDARD	VERIFIED	02:40
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:41
BLANK TEST	0.00	02:41
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	02:42
BLANK TEST	0.00	02:43
REFERENCE STANDARD TEMP	34.03c	
REFERENCE STANDARD	0.09	02:43
BLANK TEST	0.00	02:44

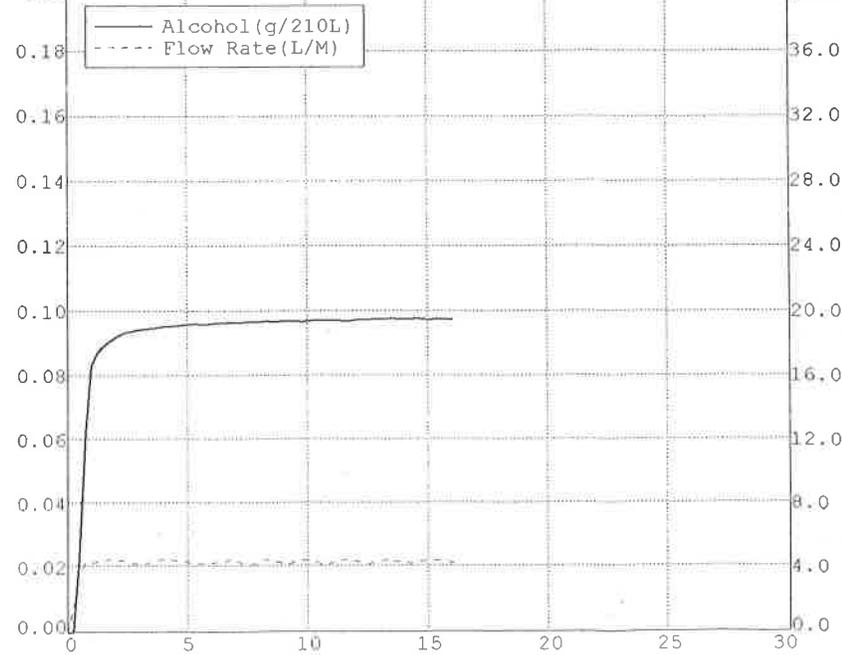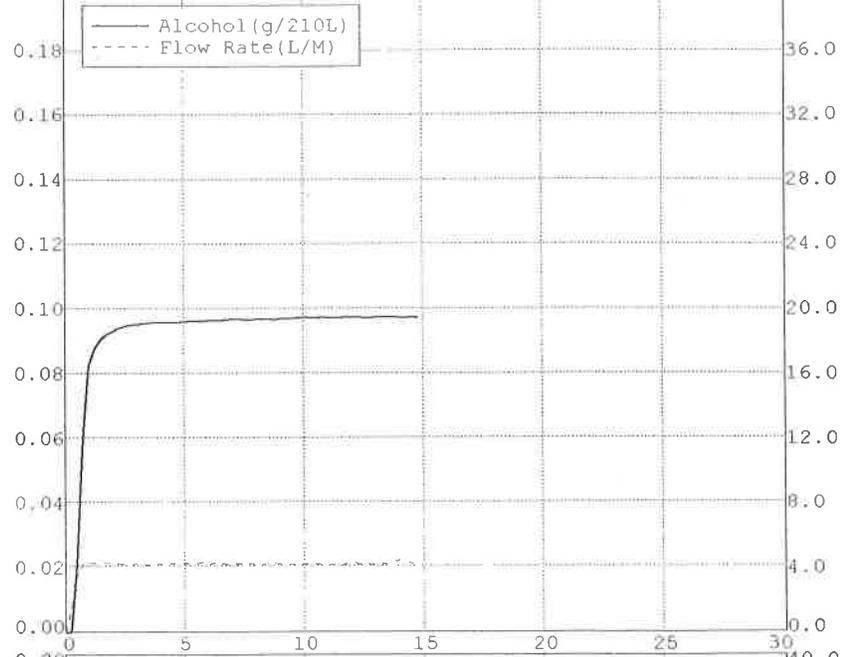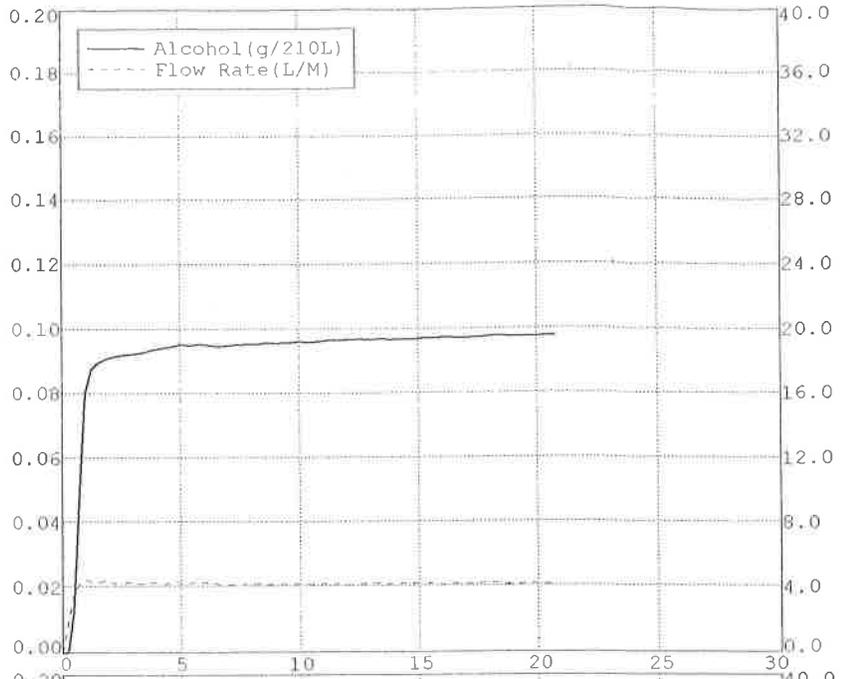

SOLUTION CHANGE

 GLENS FALLS CITY
 POLICE DEPT
 DATAMASTER dmt: 117106

Date: 02/01/2022

OPERATOR NAME:
 TYLER R MELLO
 Permit #: 46781
 Operator Agency/Dept: GLENS FALLS CITY PD
 Reference Standard #: 21440

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:07
INTERNAL STANDARD	VERIFIED	03:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	03:07
BLANK TEST	0.00	03:08
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	03:09
BLANK TEST	0.00	03:09
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	03:10
BLANK TEST	0.00	03:11

