

SUPERVISOR TEST




GLENS FALLS CITY
POLICE DEPT
DATAMASTER dmt: 117106

Date: 05/09/2022

OPERATOR NAME:
KIRSTEN M LUNDER
Permit #: 44441
Operator Agency/Dept: GLENS FALLS CITY PD
Reference Standard #: 22030

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:48
INTERNAL STANDARD	VERIFIED	04:48
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	04:48
BLANK TEST	0.00	04:49
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	04:50
BLANK TEST	0.00	04:50
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	04:51
BLANK TEST	0.00	04:52

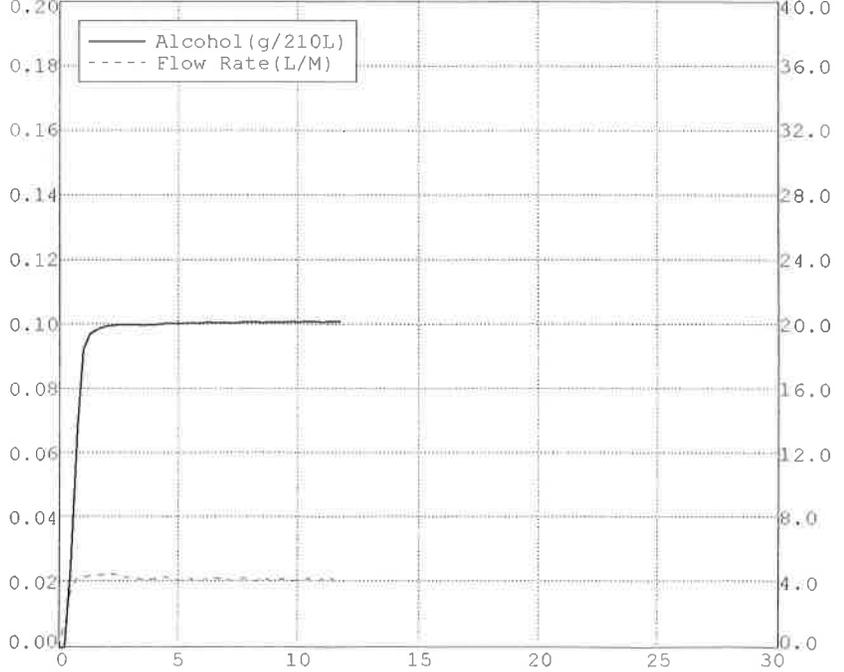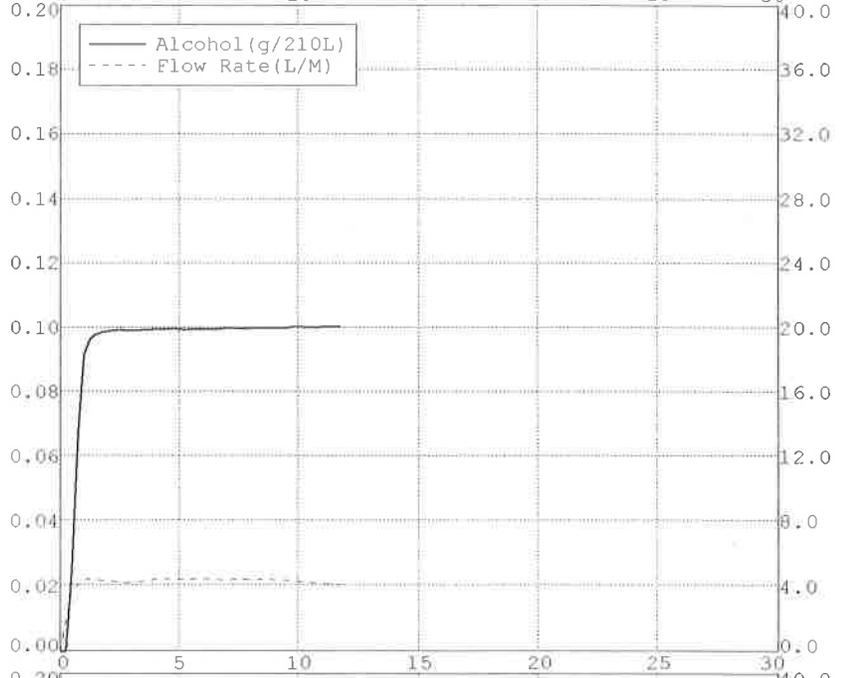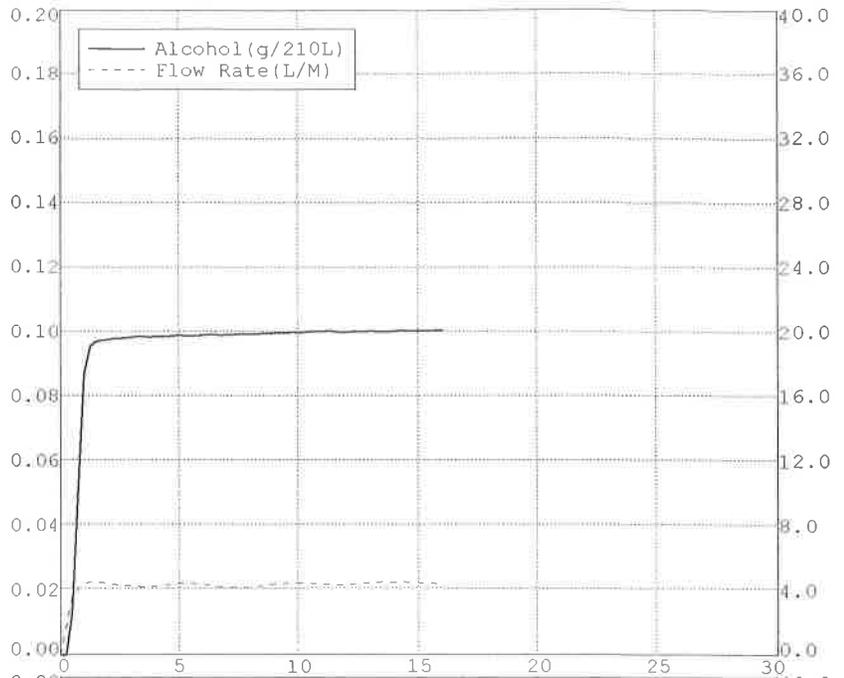

SOLUTION CHANGE

 GLENS FALLS CITY
 POLICE DEPT
 DATAMASTER dmt: 117106

Date: 05/09/2022

OPERATOR NAME:
 CARL P MATTISON
 Permit #: 42435
 Operator Agency/Dept: GLENS FALLS CITY PD
 Reference Standard #: 22030

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:50
INTERNAL STANDARD	VERIFIED	14:50
REFERENCE STANDARD TEMP	34.03c	
REFERENCE STANDARD	0.10	14:51
BLANK TEST	0.00	14:52
REFERENCE STANDARD TEMP	34.03c	
REFERENCE STANDARD	0.10	14:52
BLANK TEST	0.00	14:53
REFERENCE STANDARD TEMP	34.03c	
REFERENCE STANDARD	0.10	14:53
BLANK TEST	0.00	14:54

