

SUPERVISOR TEST



GLENS FALLS CITY
POLICE DEPT
DATAMASTER dmt: 117106

Date: 08/22/2022

OPERATOR NAME:
ROBERT M FOO
Permit #: 46059
Operator Agency/Dept: GLENS FALLS CITY PD
Reference Standard #: 22190

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:24
INTERNAL STANDARD	VERIFIED	00:24
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	00:24
BLANK TEST	0.00	00:25
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	00:25
BLANK TEST	0.00	00:26
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	00:26
BLANK TEST	0.00	00:27

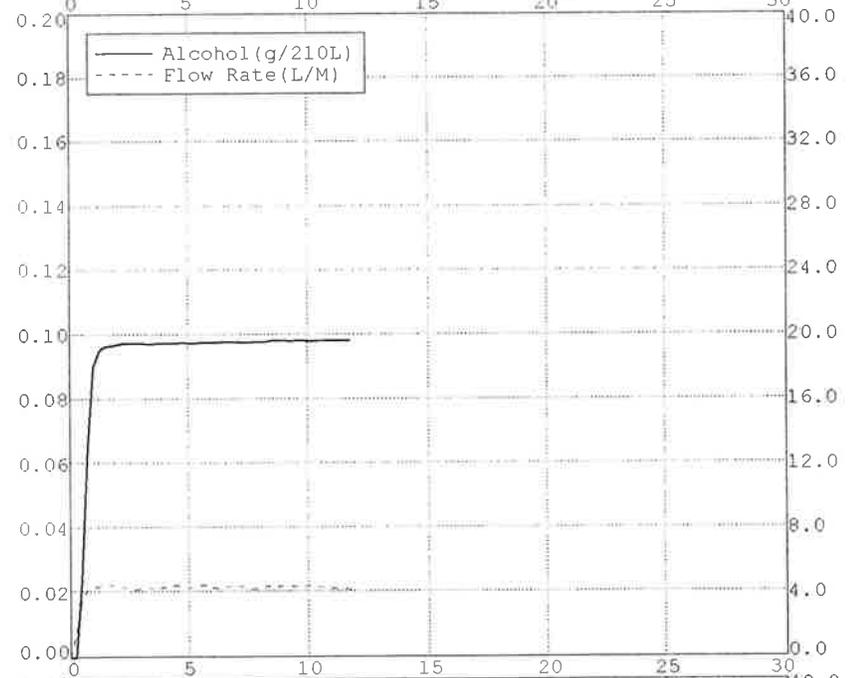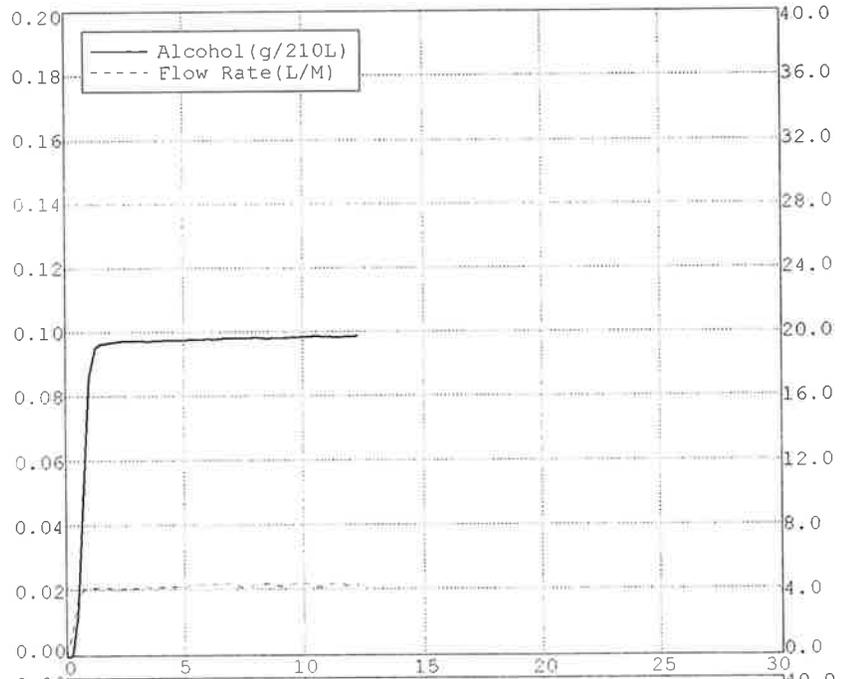

SUPERVISOR TEST

GLENS FALLS CITY
POLICE DEPT
DATAMASTER dmt: 117106

Date: 08/15/2022

OPERATOR NAME:
ROBERT M FOO
Permit #: 46059
Operator Agency/Dept: GLENS FALLS CITY PD
Reference Standard #: 22190

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:26
INTERNAL STANDARD	VERIFIED	00:26
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	00:27
BLANK TEST	0.00	00:28
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	00:28
BLANK TEST	0.00	00:29
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	00:29
BLANK TEST	0.00	00:30

