


**SIMULATOR
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Glens Falls City Police Department
Manufacturer: GUTH LABORATORIES Model: 12v500
Serial Number: MP4259
Date: May 05, 2020

Breath Simulator Temperature
34.03 degrees centigrade



Joseph Iavarone
Highway Safety Equipment Technician
Office of Public Safety

**SIMULATOR
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Glens Falls City Police Department
Manufacturer: GUTH LABORATORIES
Model: 12v500
Serial Number: MP4259
Date: May 05, 2020


1. General appearance and condition of this device -----: OK

2. Check propeller rotation -----: OK

3. Check for air leaks -----: OK

4. Check for proper temperature -----:OK

5. Record any repairs made to this instrument and list services provided: **VERIFIED CALIBRATION**

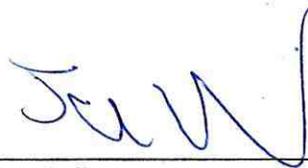

Joseph Iavarone
Highway Safety Equipment Technician
Office of Public Safety

NIST Traceable Calibration Report



1589044

Reference Number: 1376643

PO Number: MCANARY071019

NY State Division of Criminal Justice Services

80 South Swan St
HSTU 3rd Floor
Albany, NY 12210 United States

Manufacturer: Ertco
Model Number: 4400
Description: Temperature, Dig thermometer w/probe
Asset Number: 304011
Serial Number: 304011
Procedure: DS Eutechnics 4400-EP642

Calibration Date: 07/15/2019
Calibration Due Date: 07/15/2020
Condition As Found: In Tolerance
Condition As Left: In Tolerance, No adjustment

Remarks:

NIST-traceable calibration performed on the unit referenced above in accordance with customer requirements, published specifications and the lab's standard operating procedures. No adjustments were made to the unit.

Standards Utilized

Asset No.	Manufacturer	Model No.	Description	Cal. Date	Due Date
CP144317	Fluke Corporation	1595A	Thermometer, Readout, Precision Thermometer	12/16/2017	12/31/2019
CP32033	Hart Scientific	5628	Temperature, PRT- Sensor	08/22/2017	08/31/2019
CP32038	Hart Scientific	5699	Temperature, Probe, SPRT	01/18/2018	01/31/2020
CP32040	Hart Scientific	5699	Temperature, Probe, SPRT	02/12/2018	06/30/2020
CP53595	Hart Scientific	5628	Temperature, PRT- Sensor	07/30/2018	01/31/2020

Calibration Data

FUNCTION TESTED	Nominal Value	As Found	Out of Tol	As Left	Out of Tol	CALIBRATION TOLERANCE
Temperature Accuracy	-15.000 °C	-14.95		Same		-15.050 to -14.950 °C [EMU 0.013 °C][TUR 3.8:1]
	0.000 °C	0.00		Same		-0.030 to 0.030 °C [EMU 0.012 °C][TUR 2.4:1]
	75.000 °C	75.03		Same		74.970 to 75.030 °C [EMU 0.015 °C][TUR 2.0:1]
	125.000 °C	125.00		Same		124.950 to 125.050 °C [EMU 0.012 °C][TUR 4.0:1]

Temperature: 21° C
Humidity: 55% RH
Rpt. No.: 1589044

Calibration Performed By:				Quality Reviewer:	
Name	ID #	Title	Phone	Name	Date
Bautista, Arnel	358	Metrologist	847-327-5339	Pietronicco, Mike	07/15/2019

This report may not be reproduced, except in full, without written permission of Innocal. The results stated in this report relate only to the items tested or calibrated. Measurements reported herein are traceable to SI units via national standards maintained by NIST and were performed in compliance with MIL-STD-45662A, ANSI/NCSL Z540-1-1994, 10CFR50, Appendix B, ISO 9002-94, and ISO 17025:2005 Guard Banding, if reported on this certificate, is applied at a Z-factor of 30% for test points with a test uncertainty ratio (TUR) below 4:1. In Tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The estimated measurement uncertainty (EMU), if reported on this certificate, is being reported at a confidence level of 95% or K=2 unless otherwise noted in the remarks section.



New York State Division of Criminal Justice Services
SERVICE AUTHORIZATION FORM

THIS FORM IS USED TO AUTHORIZE THE DIVISION OF CRIMINAL JUSTICE SERVICES TO PERFORM SERVICE ON THE INSTRUMENT IDENTIFIED. THIS AUTHORIZATION MUST ACCOMPANY EACH PIECE OF EQUIPMENT WHEN IT IS PRESENTED TO THE EQUIPMENT REPAIR CENTER FOR SERVICE.

SECTION I - AGENCY INFORMATION

Name of Agency GLENS FALLS POLICE DEPARTMENT		Today's Date 05 MAY 2020
Address #2 RIDGE STREET		City, State, ZIP GLENS FALLS, NY 12007
Contact Person LT SHAWN LOVELACE #3930		Contact Telephone (518) 761-3840 EXT. 3782 (Desk)
Contact Telephone (518) 866-3879 (Cell)	Contact Facsimile (518) 798-4345	Contact Email slovelace@glenfallspd.com

SECTION II - INSTRUMENT INFORMATION

Instrument Manufacturer GUTH LABORATORIES INC.		Model Number 12V500
Instrument Serial Number MP 4259	Antenna Serial Number (if applicable) N/A	
Date of Malfunction 05 MAY 2020	Type of maintenance (check appropriate) <input checked="" type="checkbox"/> Calibration Check <input type="checkbox"/> Repair	
Brief Description of Malfunction YEARLY LABORATORY INSPECTION OF SIMULATOR		
List all parts, cables and/or accessories being submitted. Tuning forks must accompany all radar units. SIMULATOR WITH ASSOCIATED CABLES AND TUBES.		
I acknowledge I am signing this Service Authorization Form as an act and deed of said agency, organization, or municipality, and that I am duly authorized to sign same for the uses and purposes mentioned herein.		
Signature  #3930		Date 05 MAY 2020

DCJS USE ONLY

EXPORT 34.02°C 34.02°C 34.02°C	Digital therm 34.03°C 34.03°C 34.03°C	thpym# 304011 APP: 7/15/2020	PROPPER-OK AIR PAK CHPCR-OK
------------------------------------------------	-------------------------------------------------------	-------------------------------------------	------------------------------------------------------------