

**Infrared Instrument
Weekly Calibration Verification Test Record**

Department: Lake George Park Commission

Instrument Serial #: 300381

Test Date	Simulator Solution Lot #	Simulator Temperature			Sim. Serial#	Test Results			Breath Analysis Supervisor	Sim. Sol. Change *
		1	2	3		1	2	3		
6/17	24140	34.01	34.01	34.01	MP5081	0.09	0.09	0.09	JWW	N
6/22	24140	34.01	34.01	34.01	MP5081	0.09	0.09	0.09	JWW	N
6/30	24140	34.01	34.01	34.01	MP5081	0.09	0.09	0.09	JWW	N
7/5	24140	34.01	34.01	34.01	MP5081	0.09	0.09	0.09	JWW	Y
7/13	24140	34.01	34.01	34.01	MP5081	0.07	0.07	0.07	JWW	N
7/13	24140	34.01	34.01	34.01	MP5081	0.07	0.07	0.07	JWW	N
7/14	24140	34.01	34.01	34.01	MP5081	0.07	0.07	0.07	JWW	N
7/15	24140	34.01	34.01	34.01	MP5081	0.07	0.07	0.07	JWW	N
7/15	24190	34.01	34.01	34.01	MP5081	0.09	0.09	0.09	JWW	Y
7/20	24190	34.01	34.01	34.01	MP5081	0.09	0.09	0.09	JWW	N
7/27	24190	34.01	34.01	34.01	MP5081	0.09	0.09	0.09	JWW	N
8/2	24190	34.01	34.01	34.01	MP5081	0.09	0.09	0.09	JWW	Y

* - Please enter a √ to denote simulator solution change taking place

**Infrared Instrument
Weekly Calibration Verification Test Record**

Department: Lake George Park Commission Instrument Serial #: 300391

Test Date	Simulator Solution Lot #	Simulator Temperature			Sim. Serial#	Test Results			Breath Analysis Supervisor	Sim. Sol. Change *
		1	2	3		1	2	3		
8/10/24	24190	34.01	34.01	34.01	MP5081	0.09	0.09	0.09	JWU	N
8/17	24190	34.0	34.0	34.01	MP5081	0.09	0.09	0.09	JWU	N
8/24	24190	34.01	34.01	34.01	MP5081	0.09	0.09	0.09	JWU	N

* - Please enter a √ to denote simulator solution change taking place

SUPERVISOR TEST




LAKE GEORGE
PARK COMMISSION
DATAMASTER dmt: 300391

Date: 08/24/2024

OPERATOR NAME:
JEFFREY W WEBSTER
Permit #: 13529
Operator Agency/Dept: LAKE GEORGE PK COMM
Reference Standard #: 24190

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:58
INTERNAL STANDARD	VERIFIED	11:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	11:58
BLANK TEST	0.00	11:59
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	11:59
BLANK TEST	0.00	12:00
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	12:01
BLANK TEST	0.00	12:02

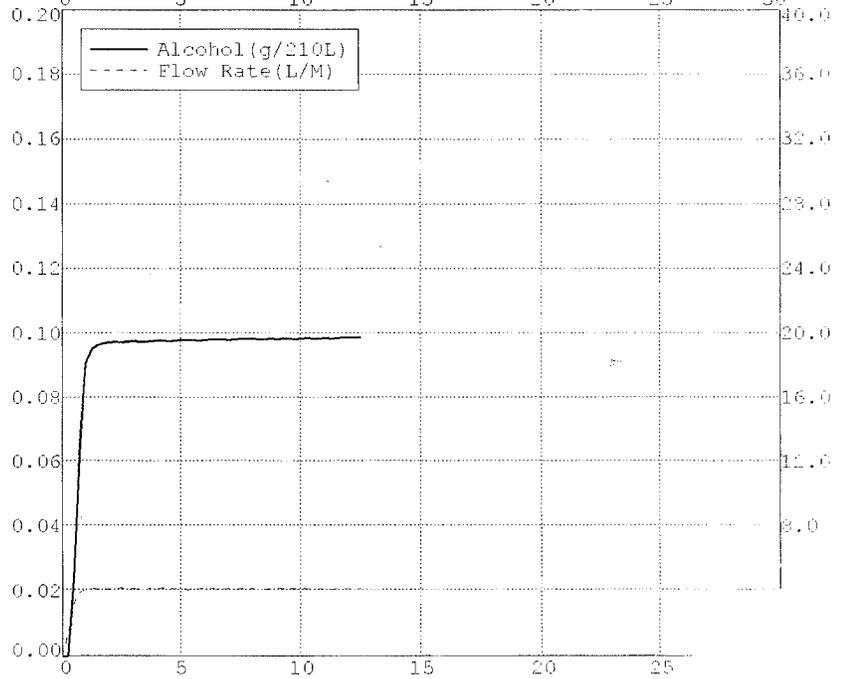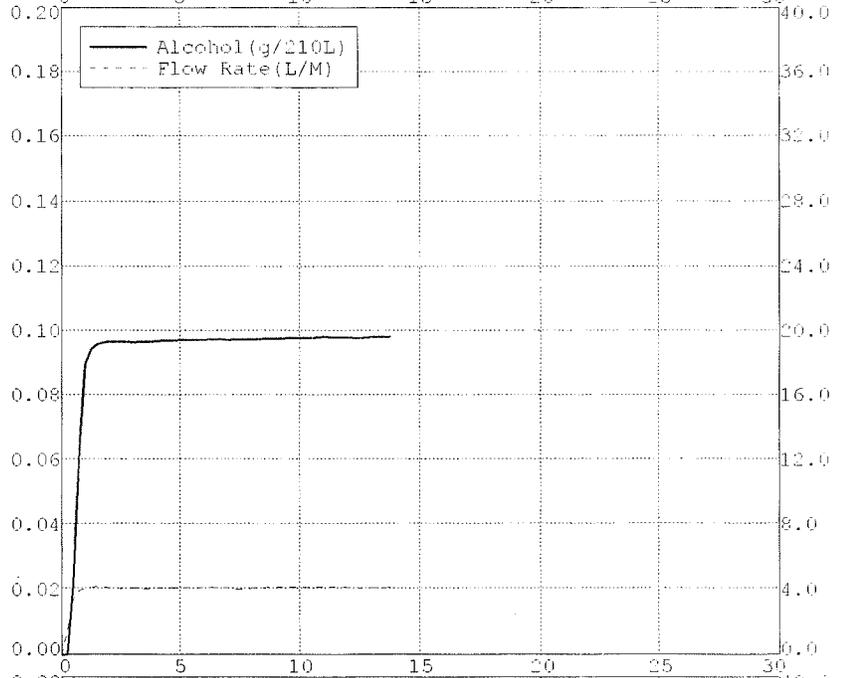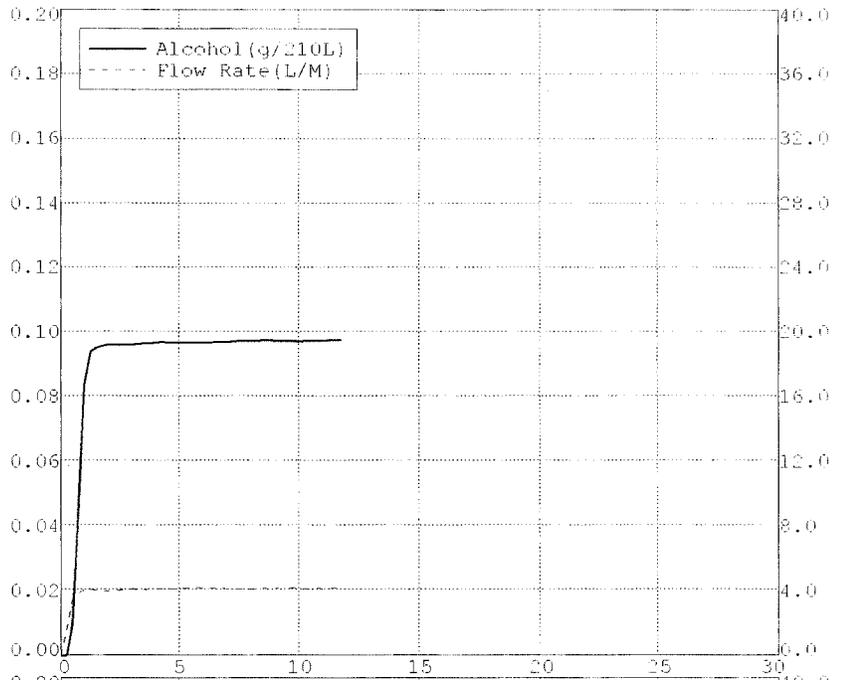

SUPERVISOR TEST




LAKE GEORGE
PARK COMMISSION
DATAMASTER dmt: 300391

Date: 08/17/2024

OPERATOR NAME:
JEFFREY W WEBSTER
Permit #: 13529
Operator Agency/Dept: LAKE GEORGE PK COMM
Reference Standard #: 24190

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:40
INTERNAL STANDARD	VERIFIED	10:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:41
BLANK TEST	0.00	10:41
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:42
BLANK TEST	0.00	10:43
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:43
BLANK TEST	0.00	10:44

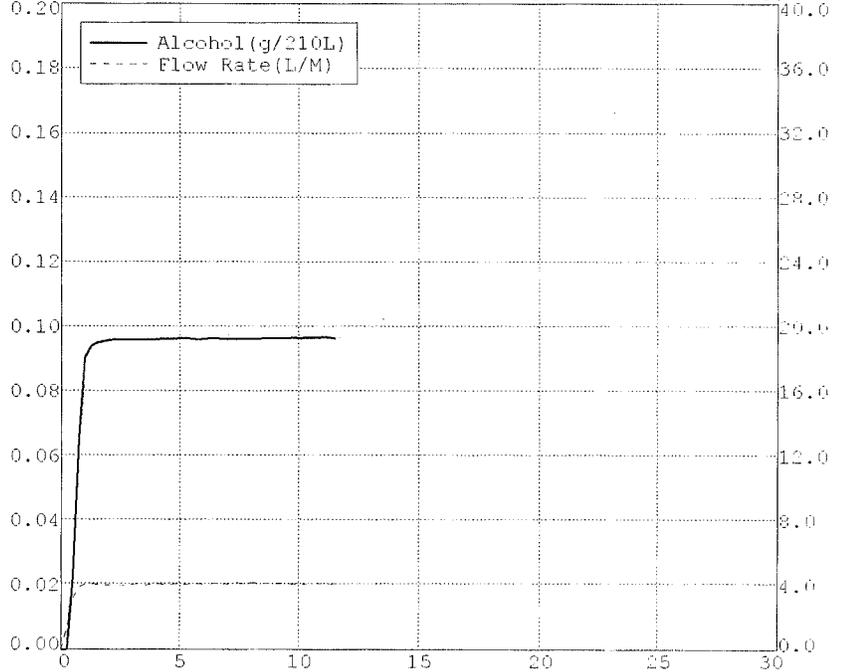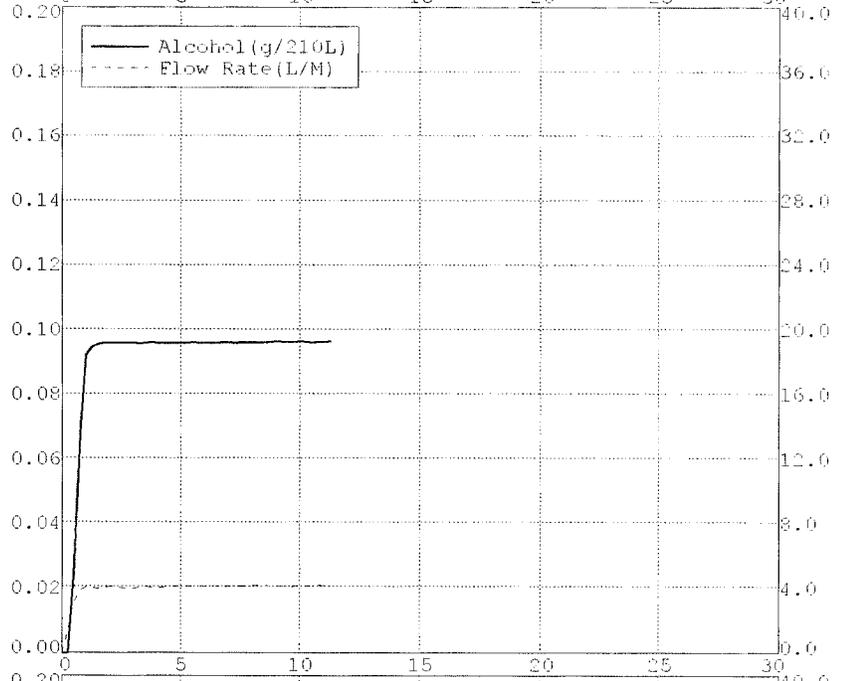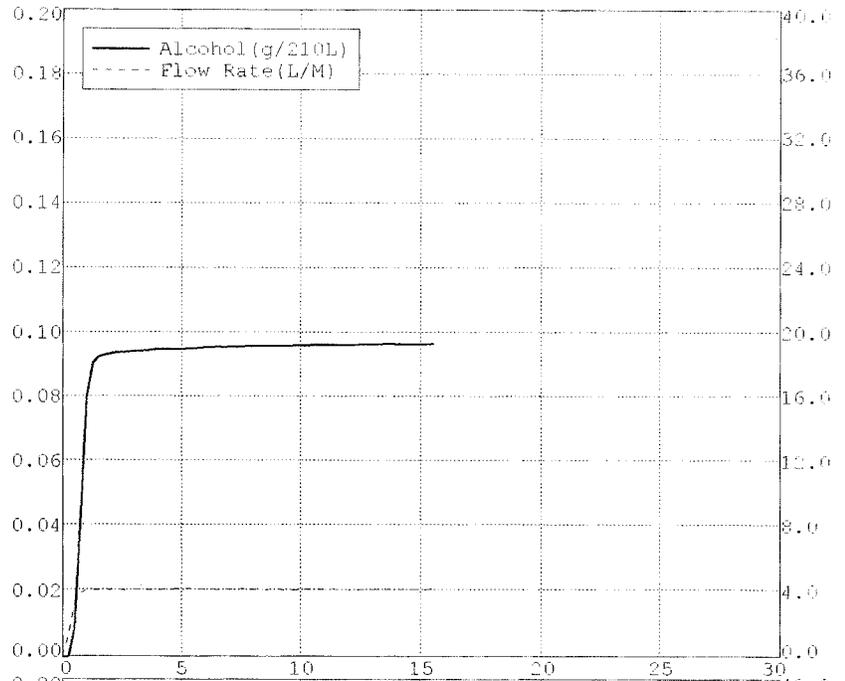

SUPERVISOR TEST




LAKE GEORGE
PARK COMMISSION
DATAMASTER dmt: 300391

Date: 08/10/2024

OPERATOR NAME:
JEFFREY W WEBSTER
Permit #: 13529
Operator Agency/Dept: LAKE GEORGE PK COMM
Reference Standard #: 24190

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:59
INTERNAL STANDARD	VERIFIED	11:59
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	11:59
BLANK TEST	0.00	12:00
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	12:00
BLANK TEST	0.00	12:01
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	12:01
BLANK TEST	0.00	12:02

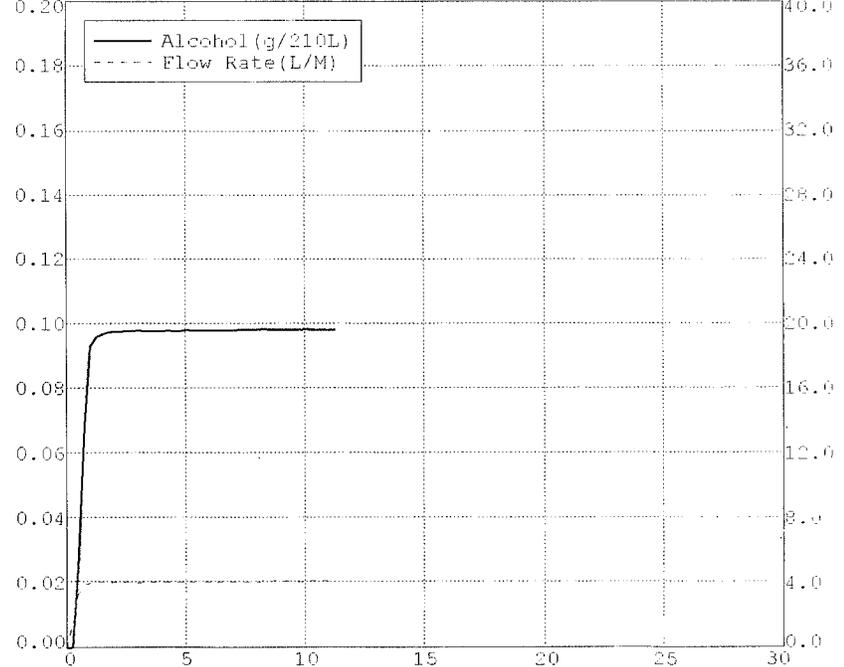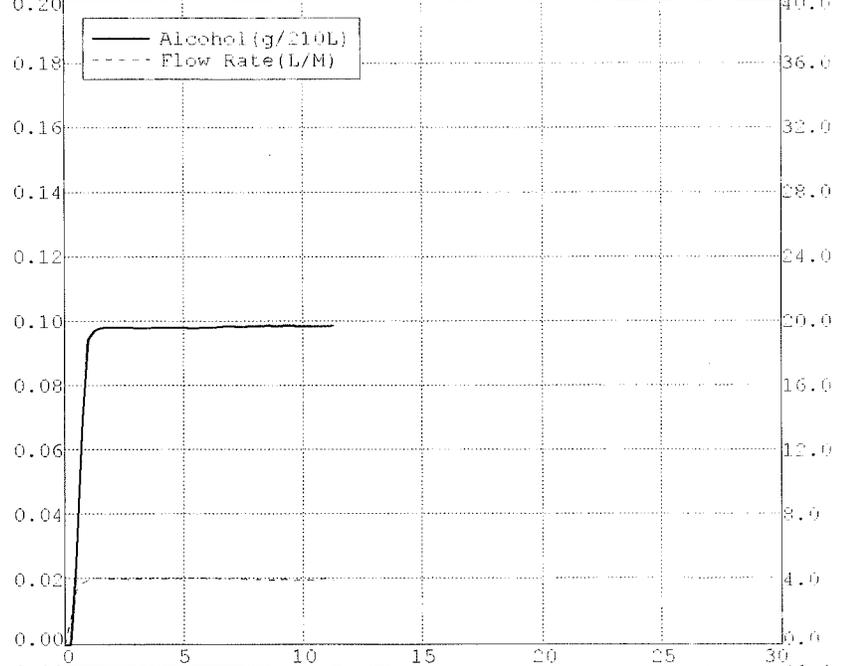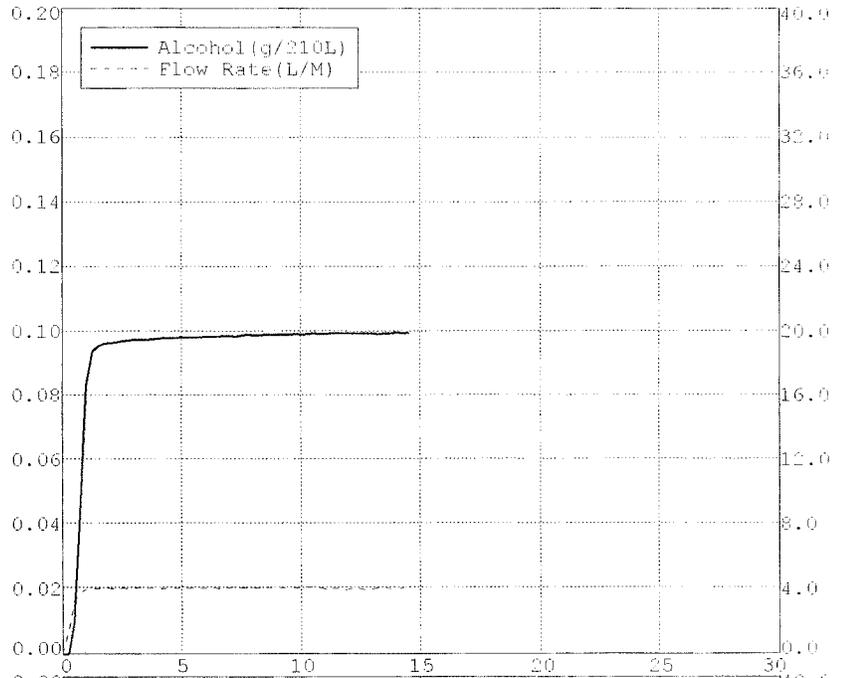

SOLUTION CHANGE




LAKE GEORGE
 PARK COMMISSION
 DATAMASTER dmt: 300391

Date: 08/02/2024

OPERATOR NAME:
 JEFFREY W WEBSTER
 Permit #: 13529
 Operator Agency/Dept: LAKE GEORGE PK COMM
 Reference Standard #: 24190

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:54
INTERNAL STANDARD	VERIFIED	12:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	12:55
BLANK TEST	0.00	12:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	12:56
BLANK TEST	0.00	12:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	12:57
BLANK TEST	0.00	12:58

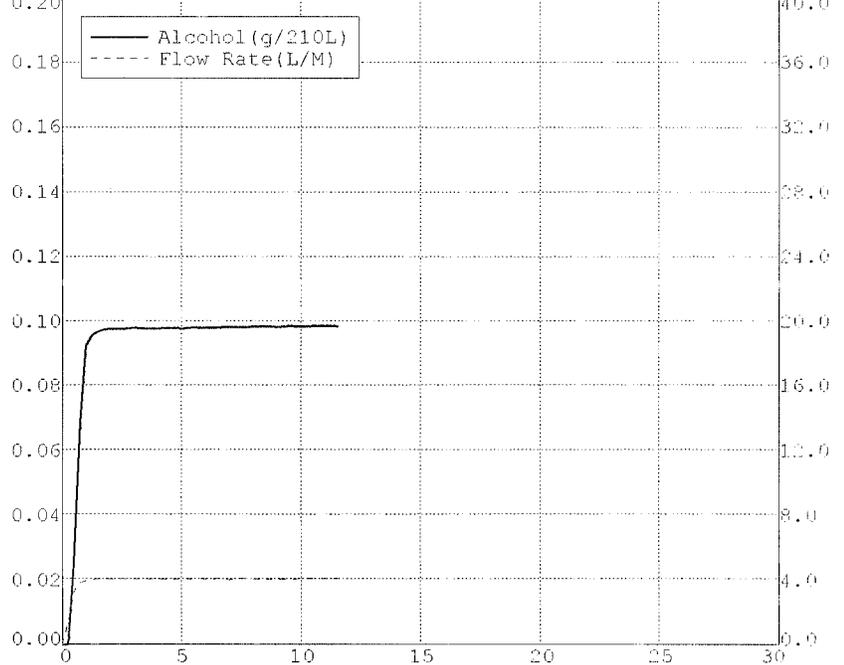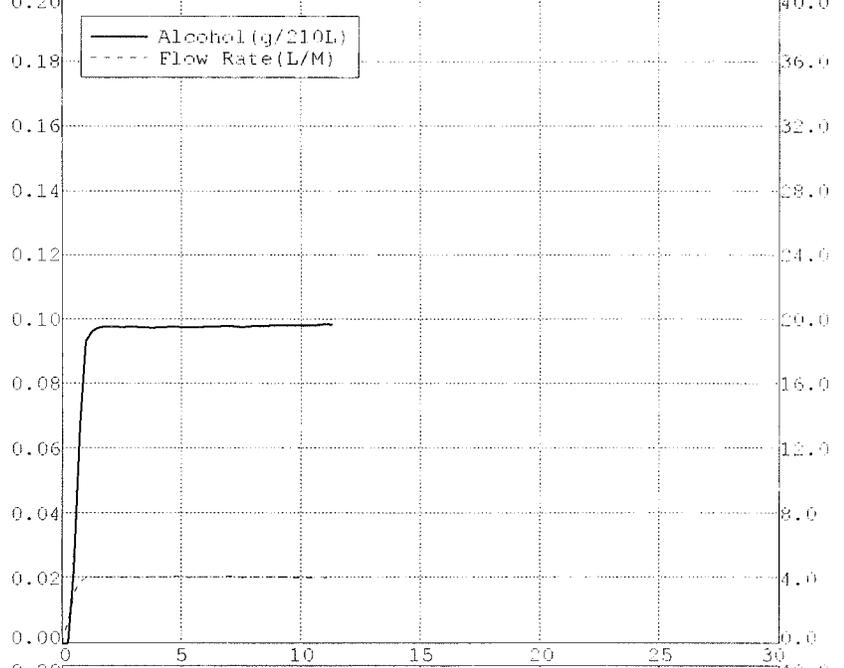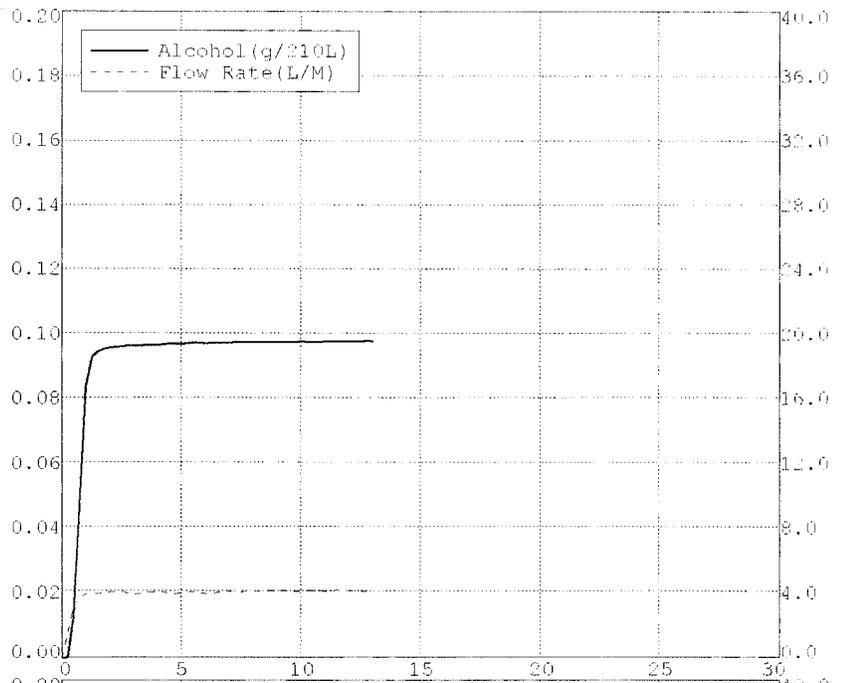

SUPERVISOR TEST




LAKE GEORGE
PARK COMMISSION
DATAMASTER dmt: 300391

Date: 07/27/2024

OPERATOR NAME:
JEFFREY W WEBSTER
Permit #: 13529
Operator Agency/Dept: LAKE GEORGE PK COMM
Reference Standard #: 24190

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:03
INTERNAL STANDARD	VERIFIED	12:03
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	12:03
BLANK TEST	0.00	12:04
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	12:04
BLANK TEST	0.00	12:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	12:06
BLANK TEST	0.00	12:06

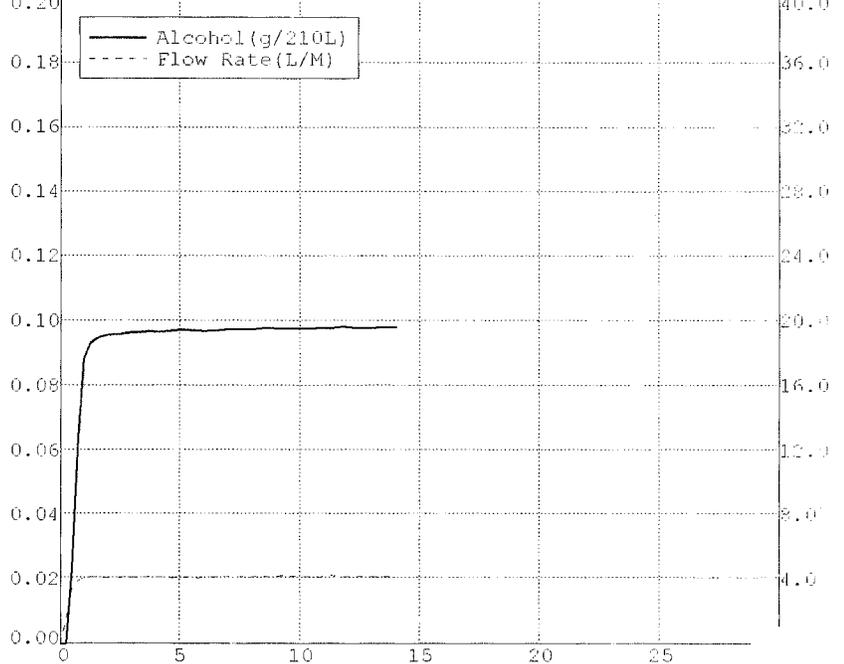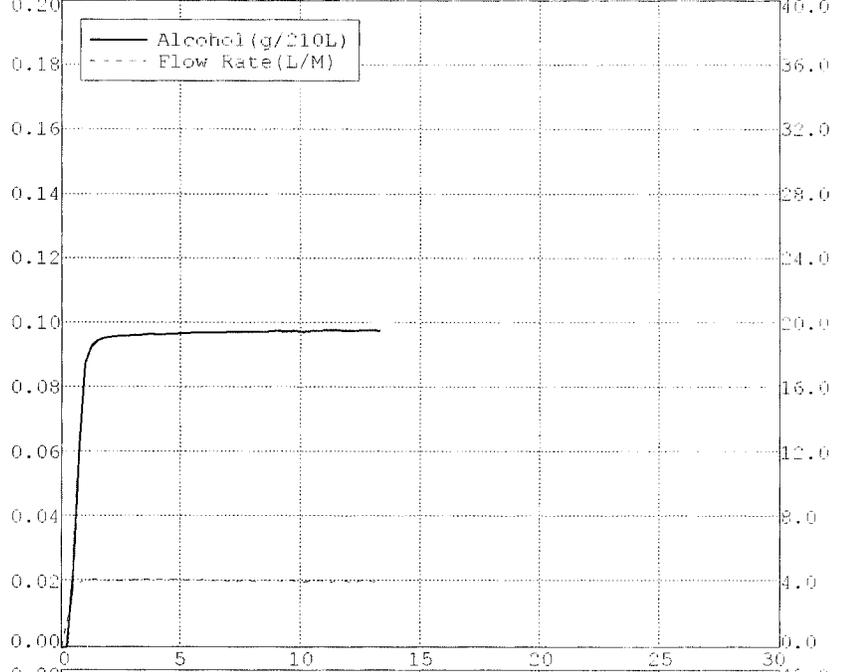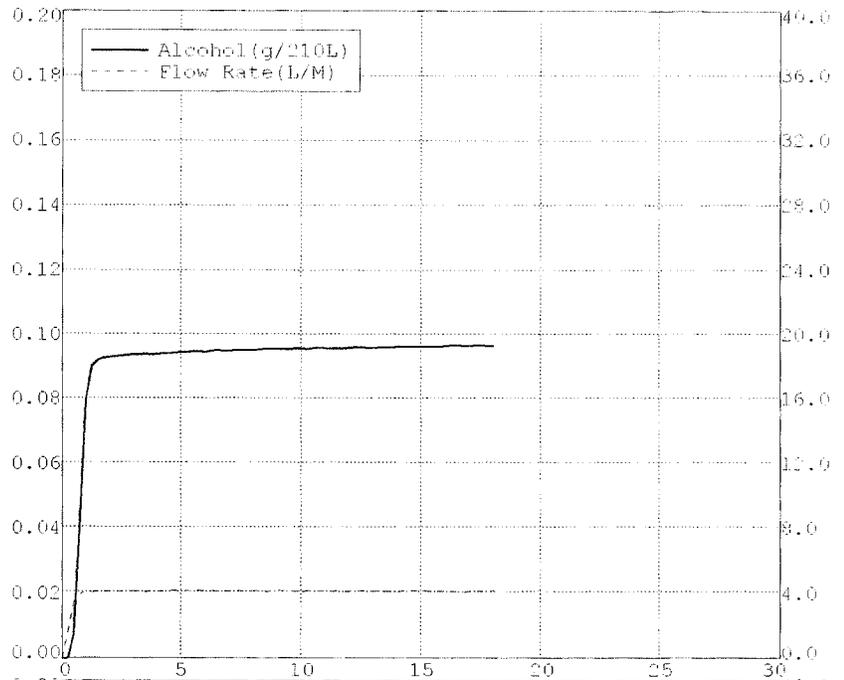

SUPERVISOR TEST




LAKE GEORGE
 PARK COMMISSION
 DATAMASTER dmt: 300391

Date: 07/20/2024

OPERATOR NAME:
 JEFFREY W WEBSTER
 Permit #: 13529
 Operator Agency/Dept: LAKE GEORGE PK COMM
 Reference Standard #: 24190

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:56
INTERNAL STANDARD	VERIFIED	11:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	11:56
BLANK TEST	0.00	11:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	11:57
BLANK TEST	0.00	11:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	11:58
BLANK TEST	0.00	11:59

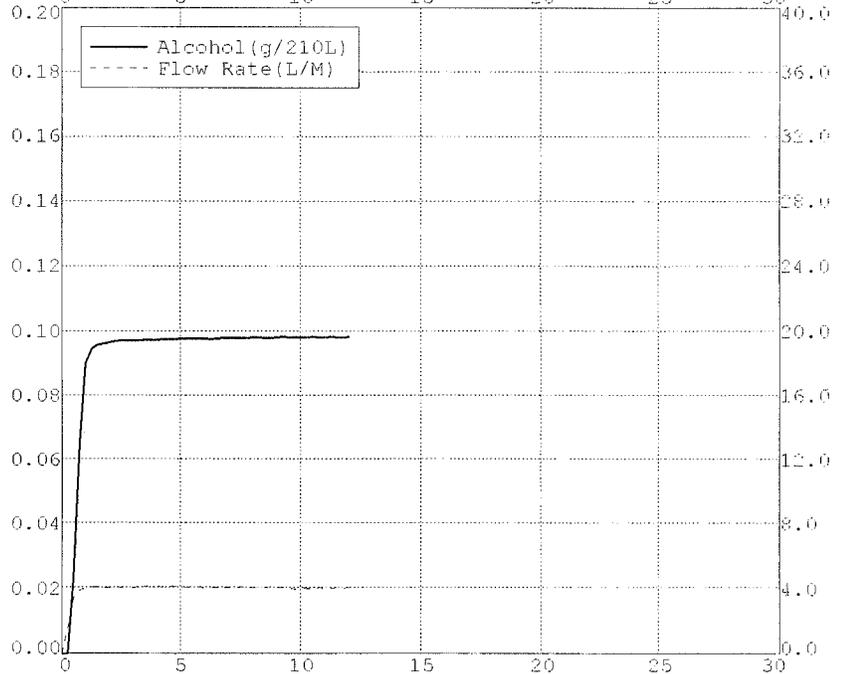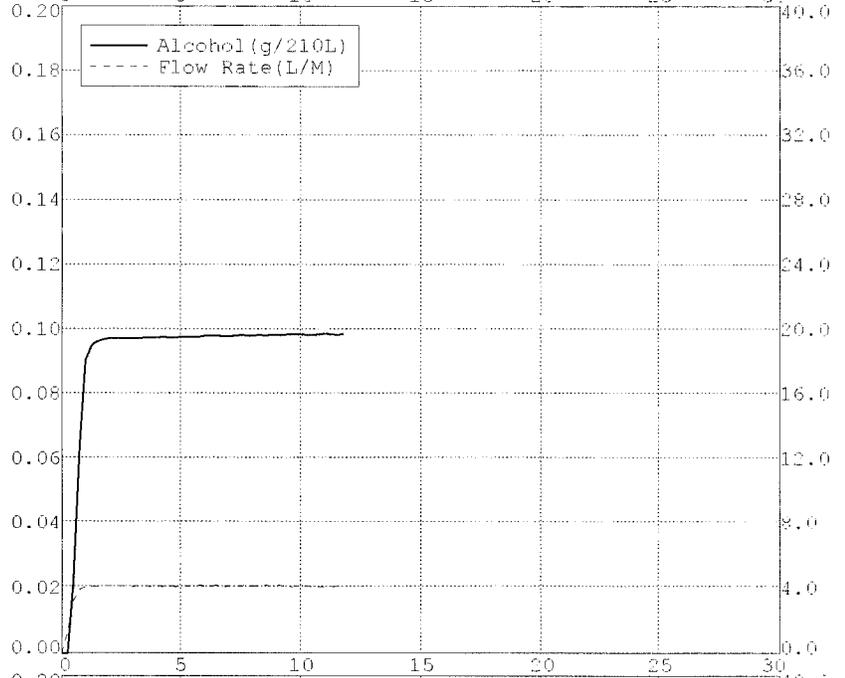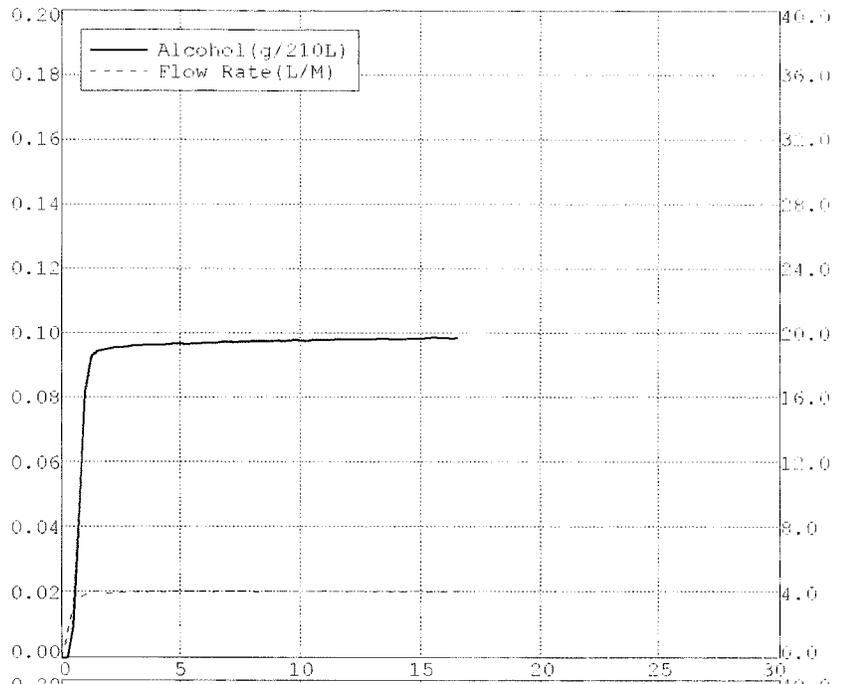

SOLUTION CHANGE




LAKE GEORGE
 PARK COMMISSION
 DATAMASTER dmt: 300391

Date: 07/15/2024

OPERATOR NAME:
 JEFFREY W WEBSTER
 Permit #: 13529
 Operator Agency/Dept: LAKE GEORGE PK COMM
 Reference Standard #: 24190

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:46
INTERNAL STANDARD	VERIFIED	19:46
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	19:46
BLANK TEST	0.00	19:47
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	19:47
BLANK TEST	0.00	19:48
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	19:48
BLANK TEST	0.00	19:49

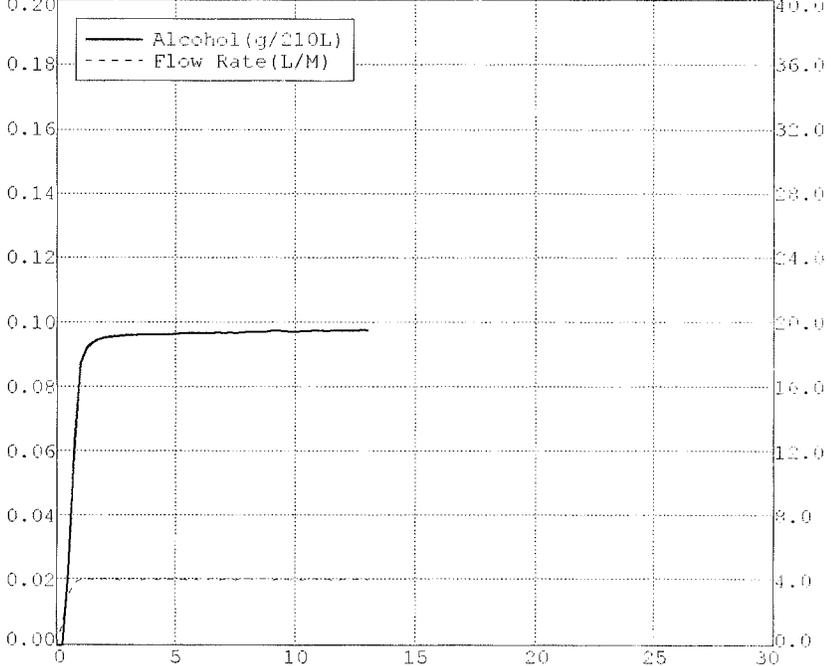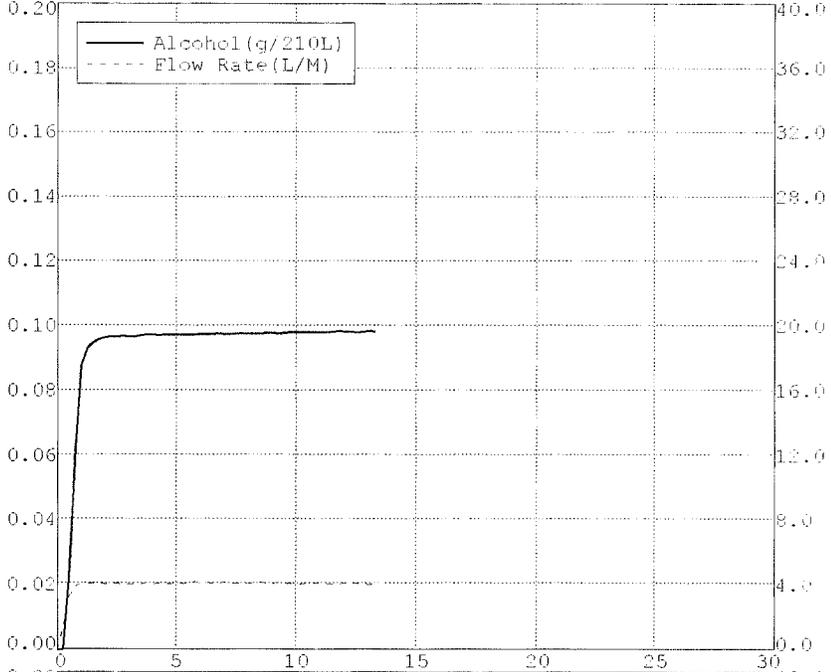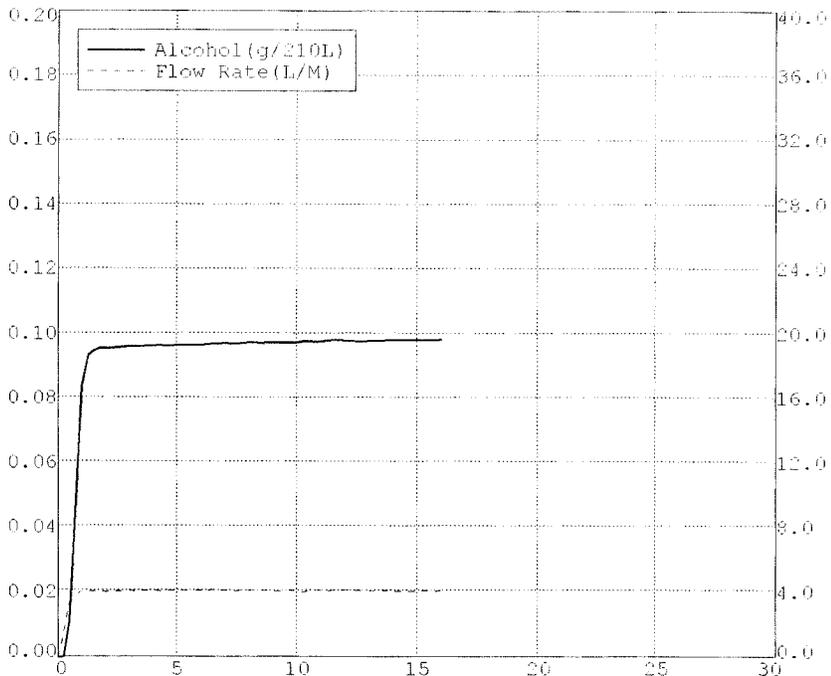

SUPERVISOR TEST




LAKE GEORGE
PARK COMMISSION
DATAMASTER dmt: 300391

Date: 07/15/2024

OPERATOR NAME:
JEFFREY W WEBSTER
Permit #: 13529
Operator Agency/Dept: LAKE GEORGE PK COMM
Reference Standard #: 24140

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:21
INTERNAL STANDARD	VERIFIED	10:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.07	10:22
BLANK TEST	0.00	10:23
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.07	10:23
BLANK TEST	0.00	10:24
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.07	10:24
BLANK TEST	0.00	10:25

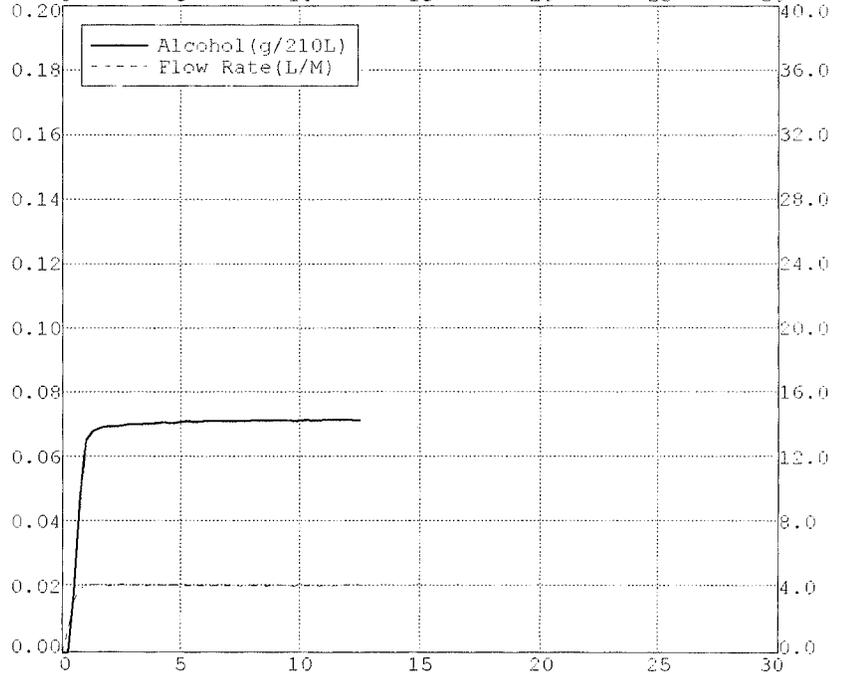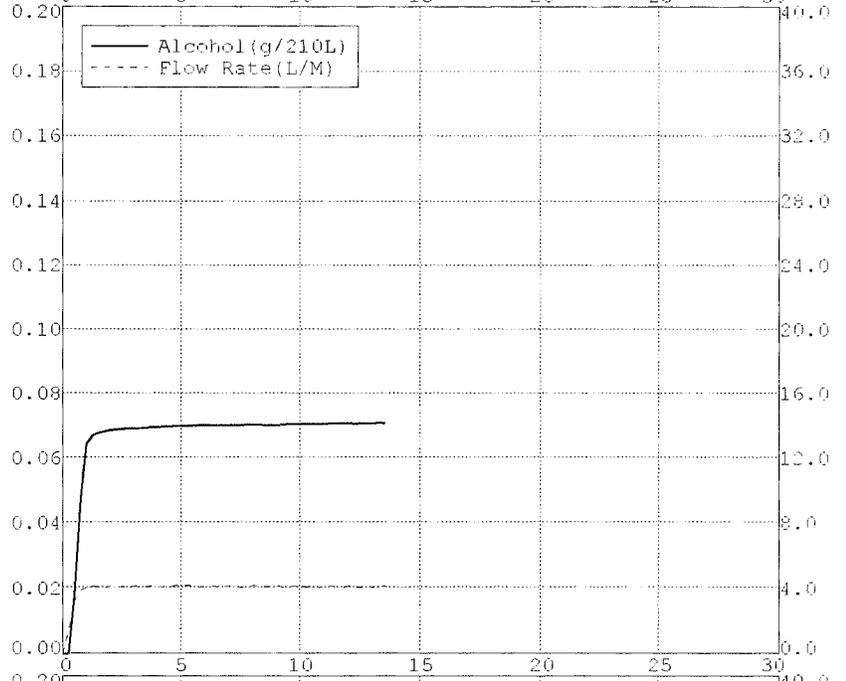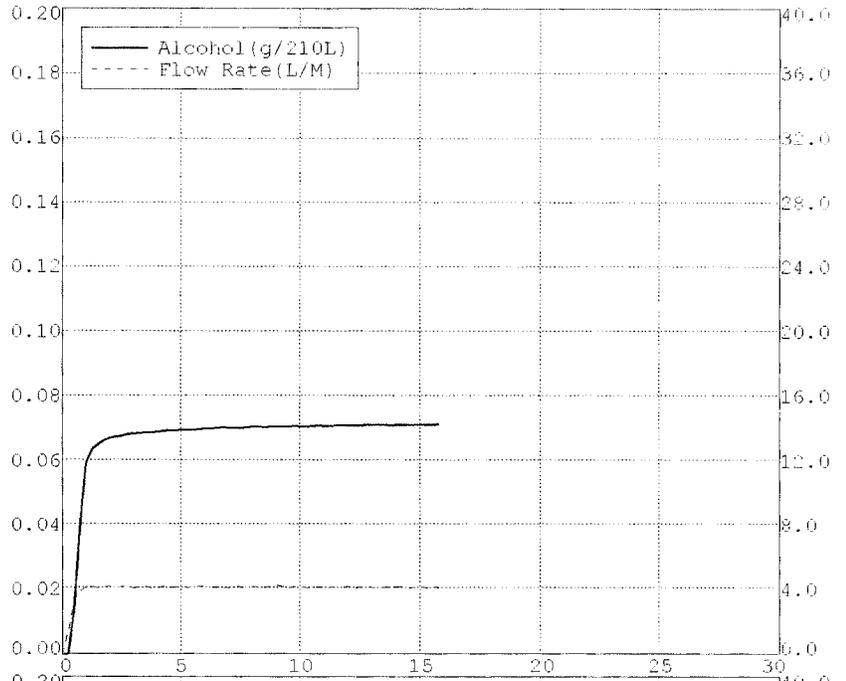

SUPERVISOR TEST



LAKE GEORGE
PARK COMMISSION
DATAMASTER dmt: 300391

Date: 07/15/2024

OPERATOR NAME:
JEFFREY W WEBSTER
Permit #: 13529
Operator Agency/Dept: LAKE GEORGE PK COMM
Reference Standard #: 24140

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:05
INTERNAL STANDARD	VERIFIED	10:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.07	10:06
BLANK TEST	0.00	10:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.07	10:07
BLANK TEST	0.00	10:08
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.07	10:08
BLANK TEST	0.00	10:09

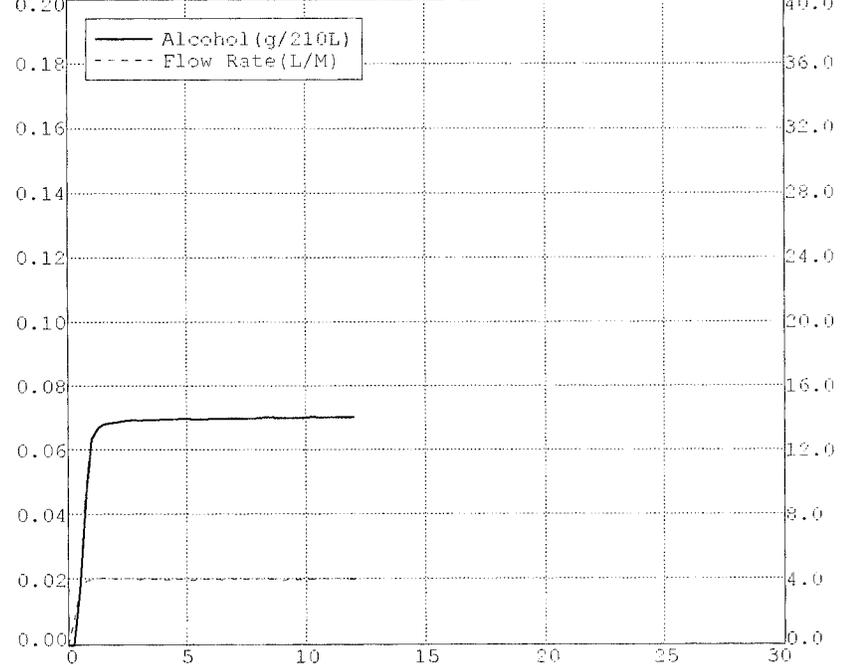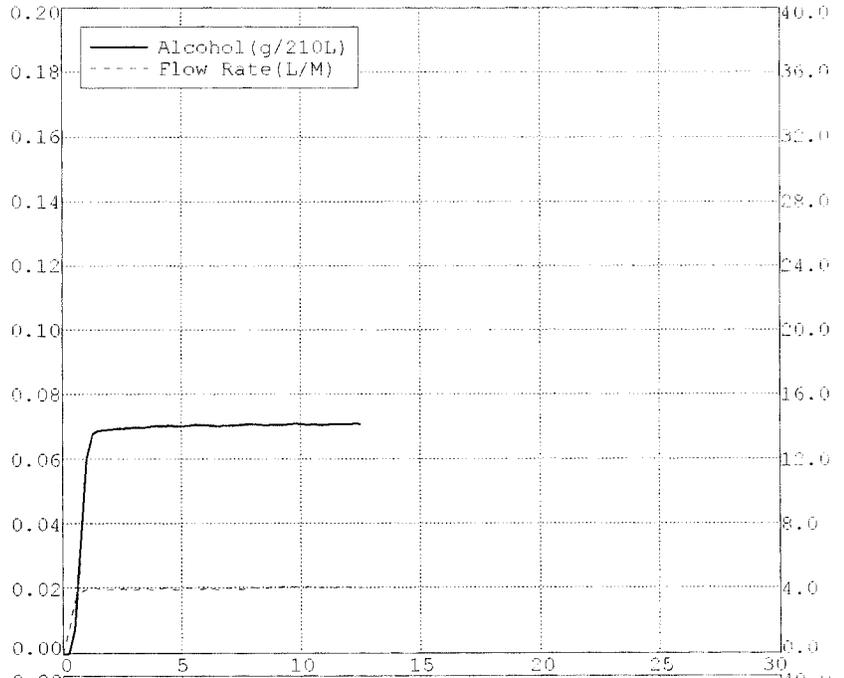

SUPERVISOR TEST




LAKE GEORGE
PARK COMMISSION
DATAMASTER dmt: 300391

Date: 07/15/2024

OPERATOR NAME:
JEFFREY W WEBSTER
Permit #: 13529
Operator Agency/Dept: LAKE GEORGE PK COMM
Reference Standard #: 24140

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:12
INTERNAL STANDARD	VERIFIED	10:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.07	10:12
BLANK TEST	0.00	10:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.07	10:13
BLANK TEST	0.00	10:14
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.07	10:14
BLANK TEST	0.00	10:15

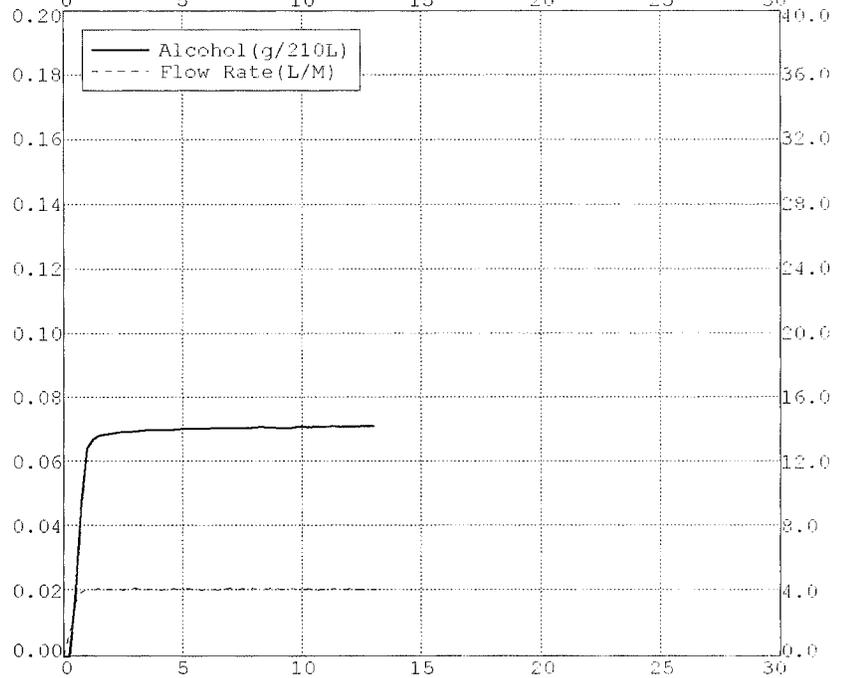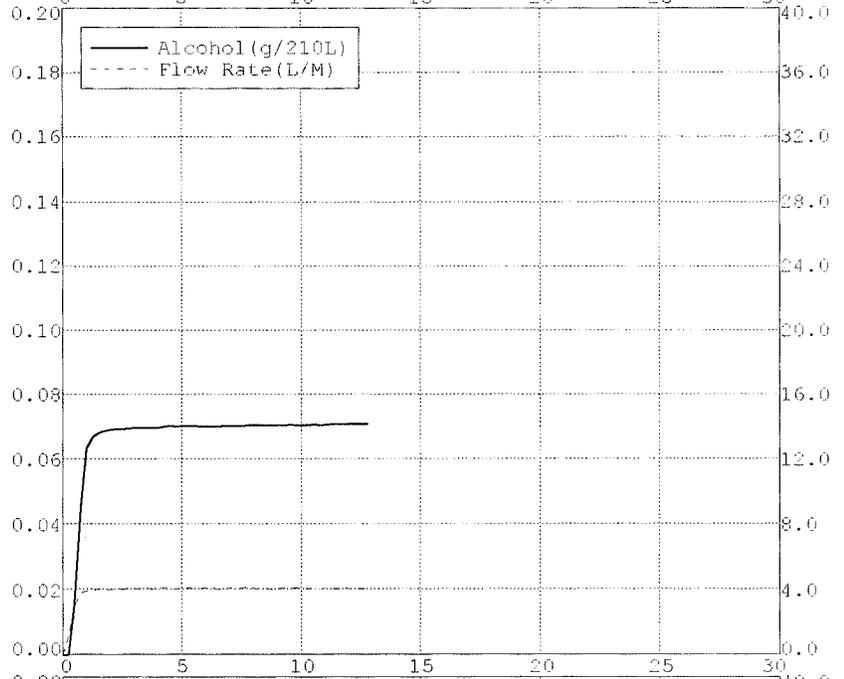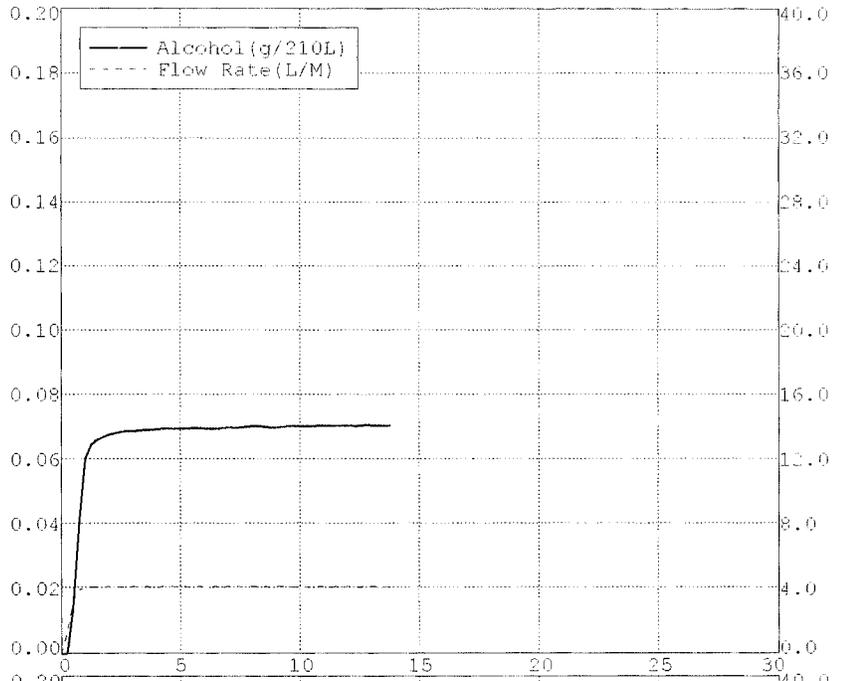

SUPERVISOR TEST




LAKE GEORGE
 PARK COMMISSION
 DATAMASTER dmt: 300391

Date: 07/14/2024

OPERATOR NAME:
 ANGELO P PACCIONE
 Permit #: 47655
 Operator Agency/Dept: LAKE GEORGE PK COMM
 Reference Standard #: 24140

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:55
INTERNAL STANDARD	VERIFIED	10:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.07	10:56
BLANK TEST	0.00	10:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.07	10:57
BLANK TEST	0.00	10:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.06	10:58
BLANK TEST	0.00	10:59

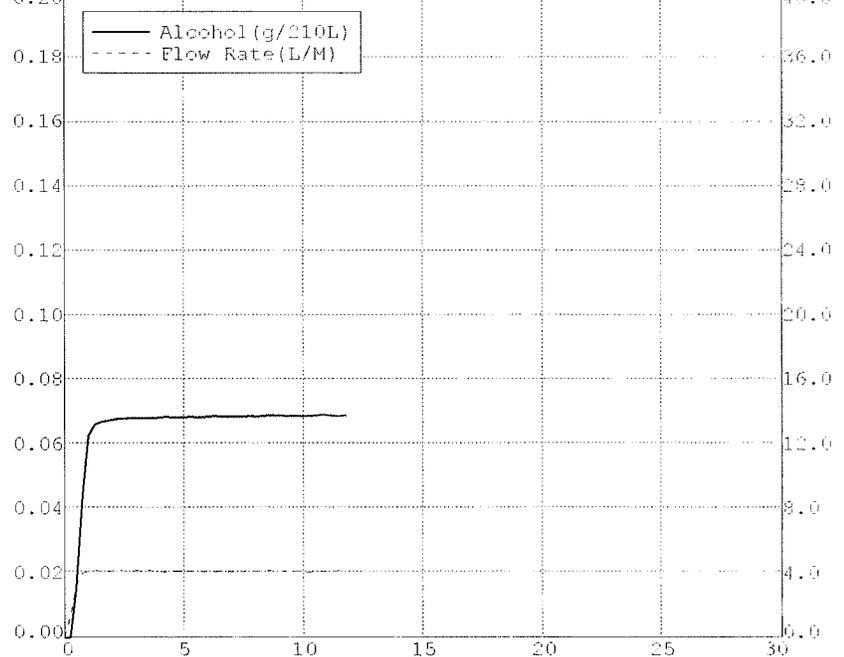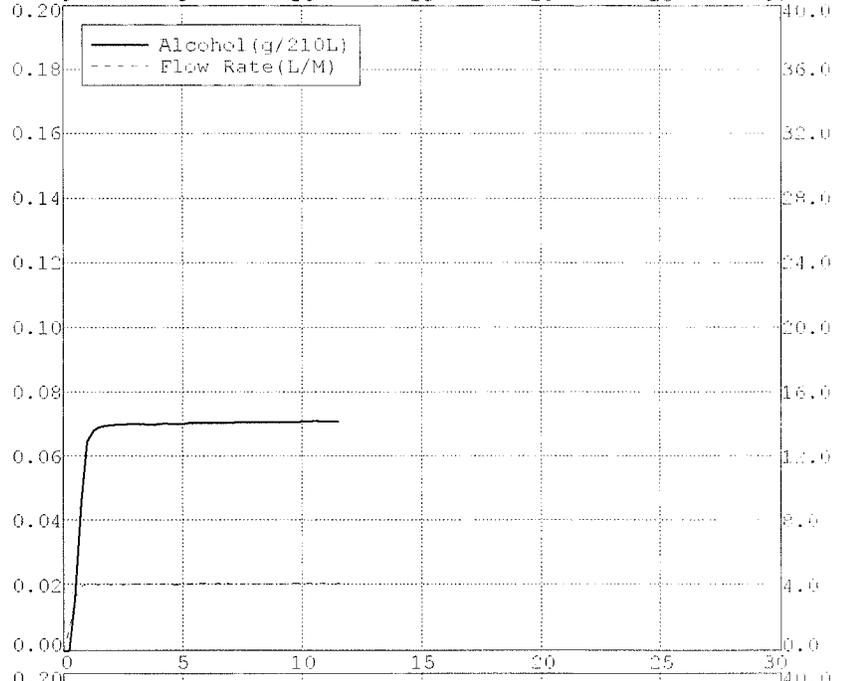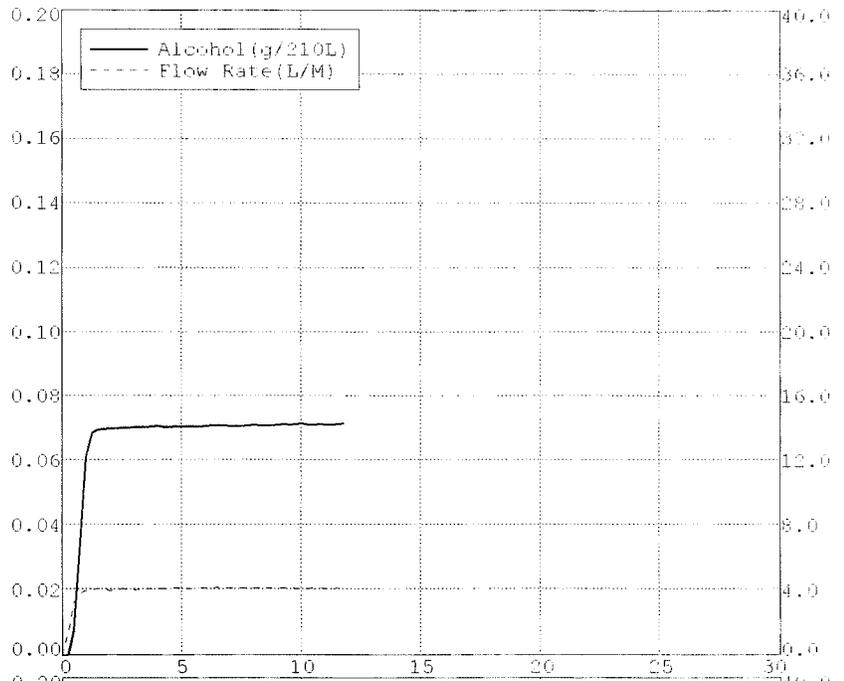

SUPERVISOR TEST




LAKE GEORGE
PARK COMMISSION
DATAMASTER dmt: 300391

Date: 07/13/2024

OPERATOR NAME:
JEFFREY W WEBSTER
Permit #: 13529
Operator Agency/Dept: LAKE GEORGE PK COMM
Reference Standard #: 24140

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:56
INTERNAL STANDARD	VERIFIED	13:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.07	13:57
BLANK TEST	0.00	13:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.07	13:58
BLANK TEST	0.00	13:59
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.07	13:59
BLANK TEST	0.00	14:00

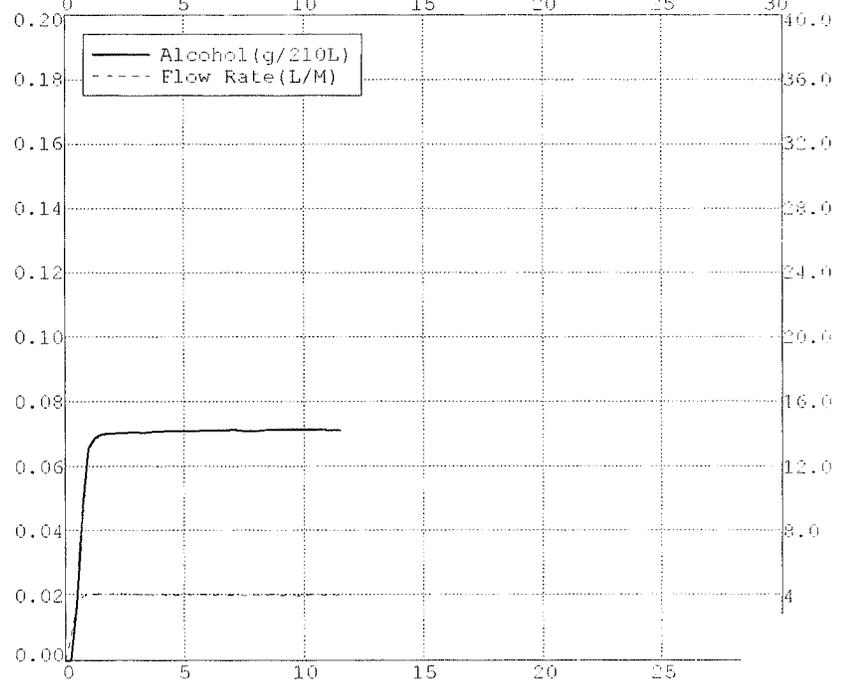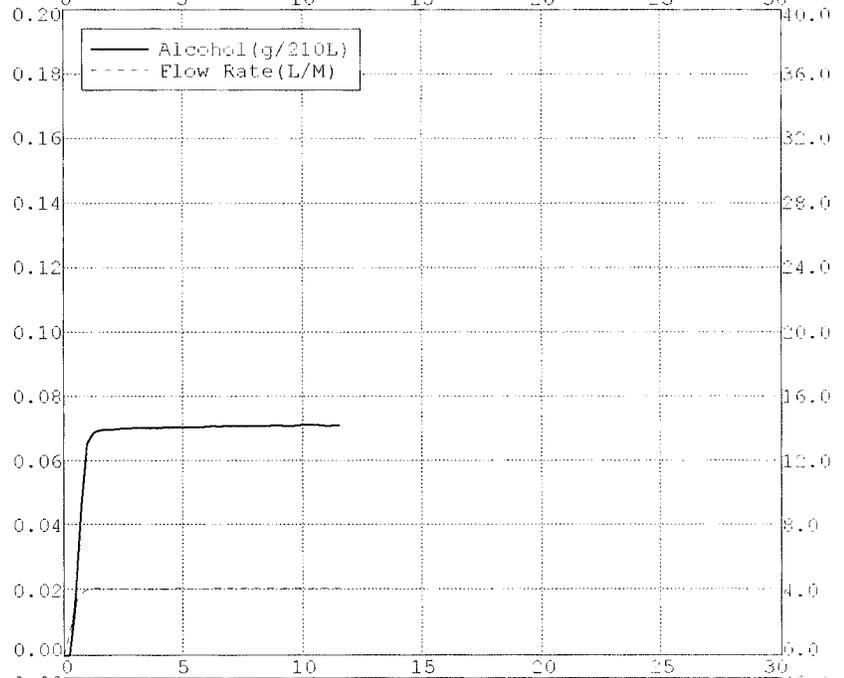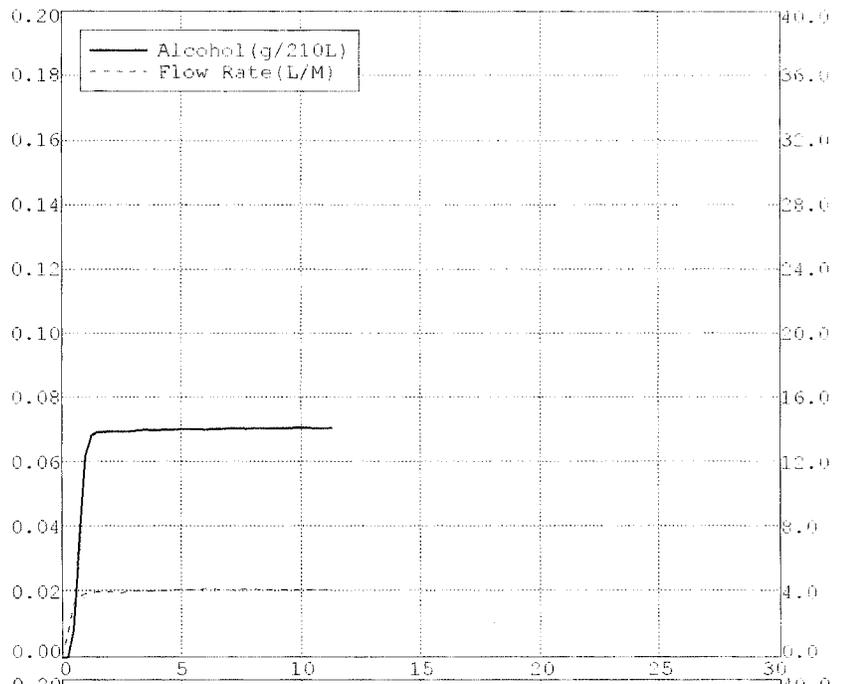

SUPERVISOR TEST




LAKE GEORGE
PARK COMMISSION
DATAMASTER dmt: 300391

Date: 07/13/2024

OPERATOR NAME:
JEFFREY W WEBSTER
Permit #: 13529
Operator Agency/Dept: LAKE GEORGE PK COMM
Reference Standard #: 24140

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:00
INTERNAL STANDARD	VERIFIED	12:00
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.07	12:01
BLANK TEST	0.00	12:02
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.07	12:02
BLANK TEST	0.00	12:03
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.07	12:03
BLANK TEST	0.00	12:04

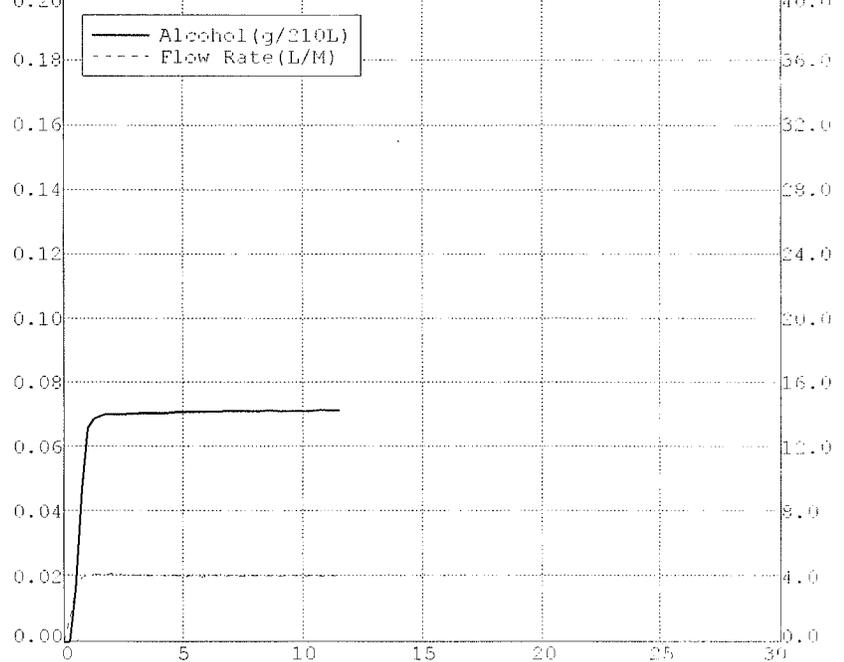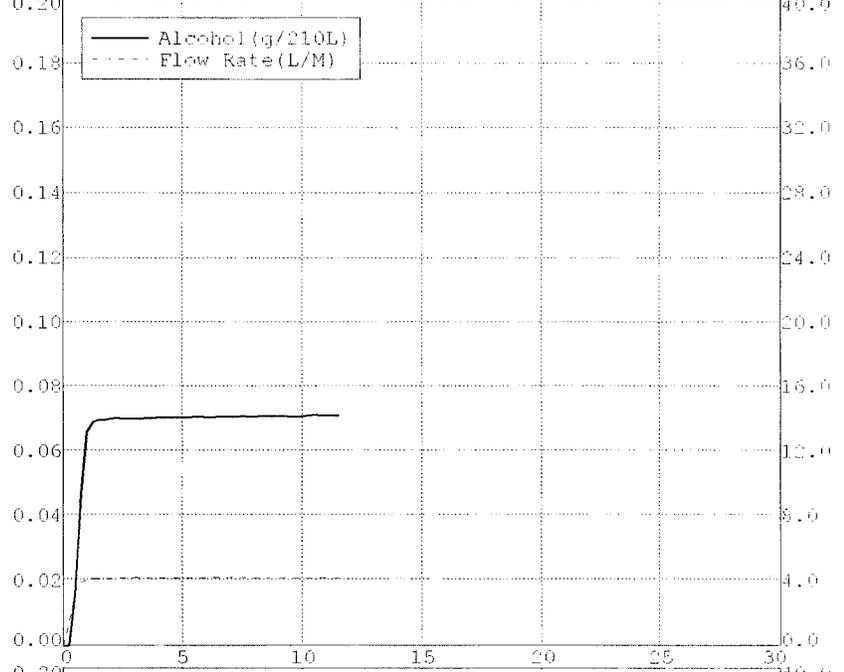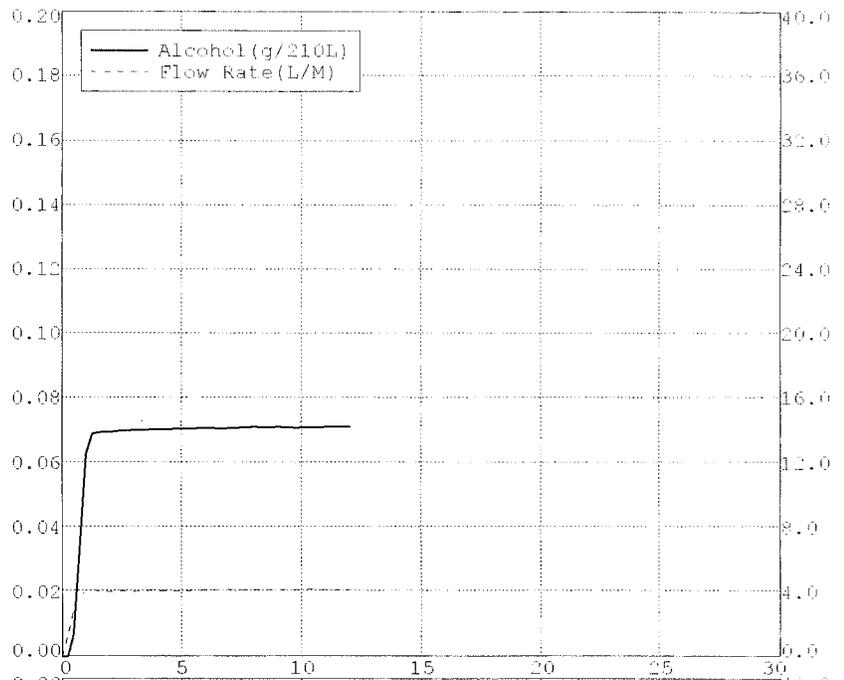

SOLUTION CHANGE




LAKE GEORGE
PARK COMMISSION
DATAMASTER dmt: 300391

Date: 07/06/2024

OPERATOR NAME:
JEFFREY W WEBSTER
Permit #: 13529
Operator Agency/Dept: LAKE GEORGE PK COMM
Reference Standard #: 24140

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:01
INTERNAL STANDARD	VERIFIED	13:01
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:02
BLANK TEST	0.00	13:03
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:03
BLANK TEST	0.00	13:04
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:04
BLANK TEST	0.00	13:05

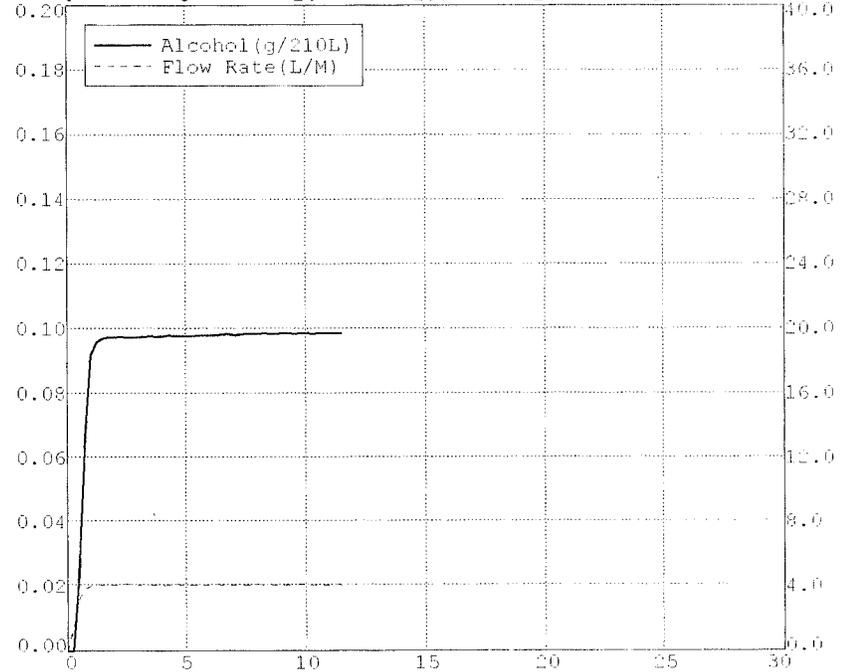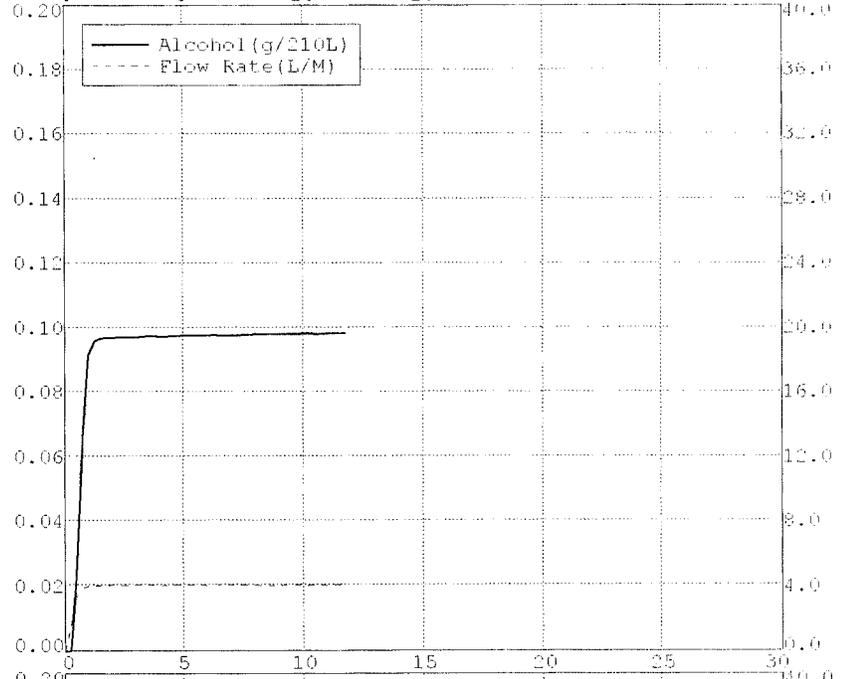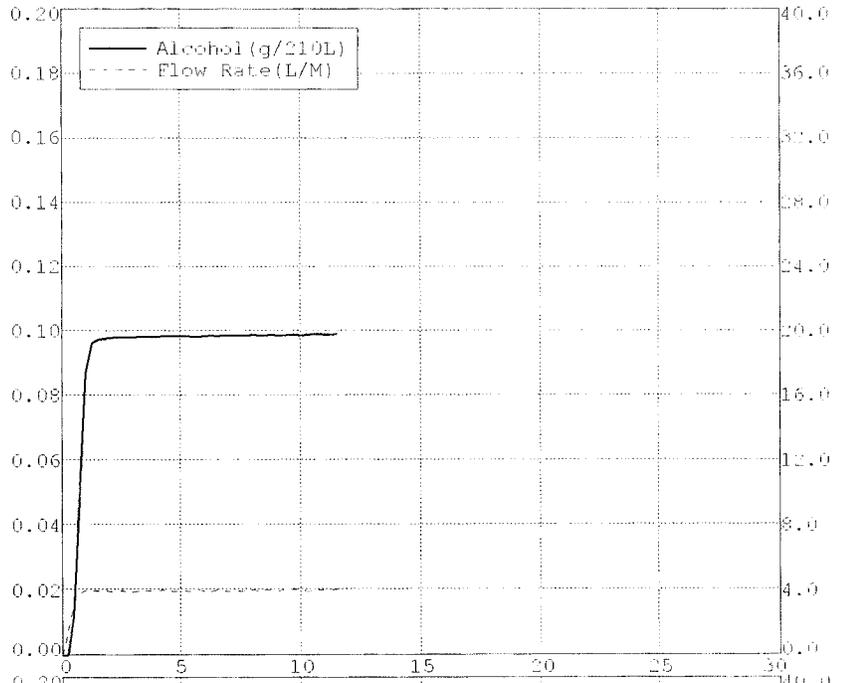

SUPERVISOR TEST




LAKE GEORGE
PARK COMMISSION
DATAMASTER dmt: 300391

Date: 06/30/2024

OPERATOR NAME:
JEFFREY W WEBSTER
Permit #: 13529
Operator Agency/Dept: LAKE GEORGE PK COMM
Reference Standard #: 24140

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:08
INTERNAL STANDARD	VERIFIED	10:08
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:09
BLANK TEST	0.00	10:09
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:10
BLANK TEST	0.00	10:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:11
BLANK TEST	0.00	10:12

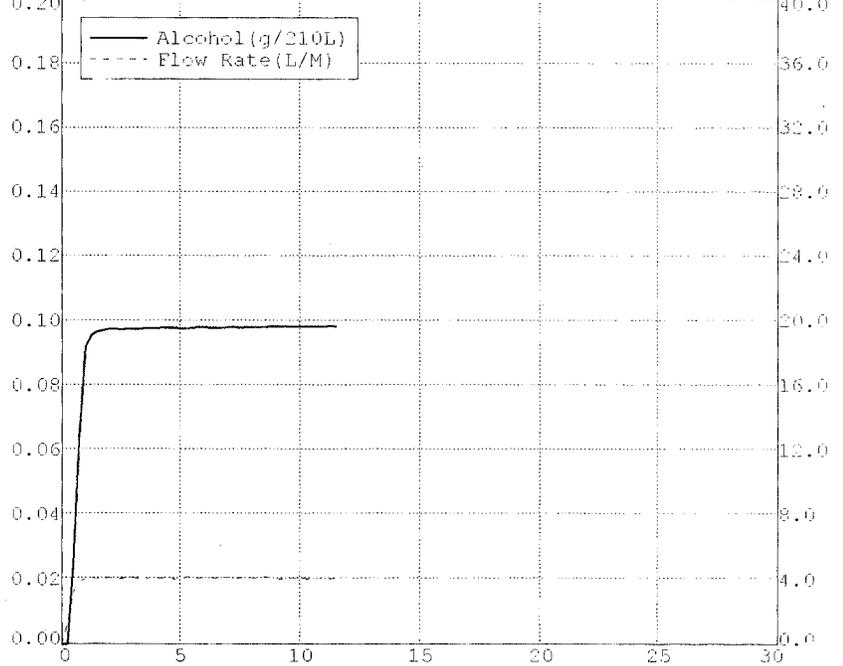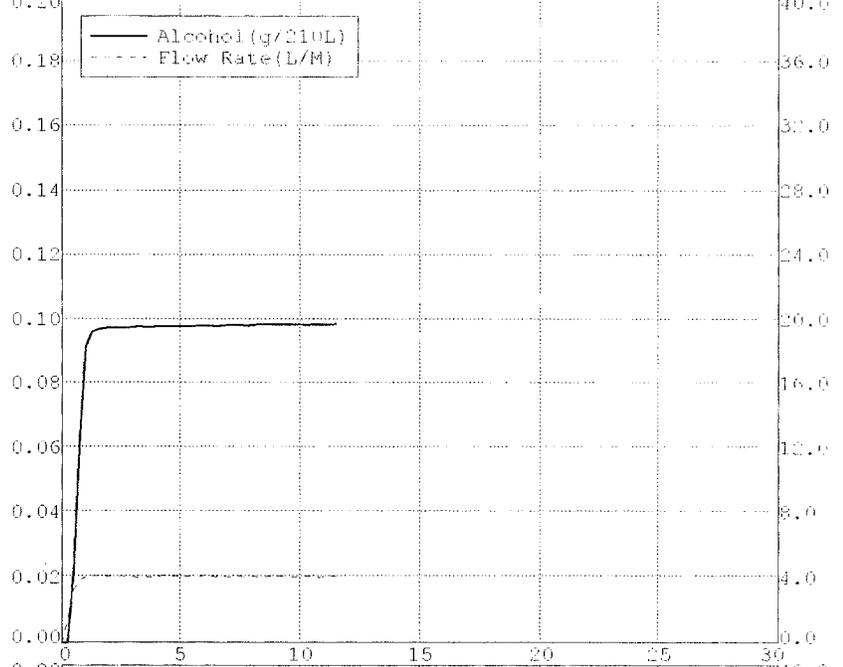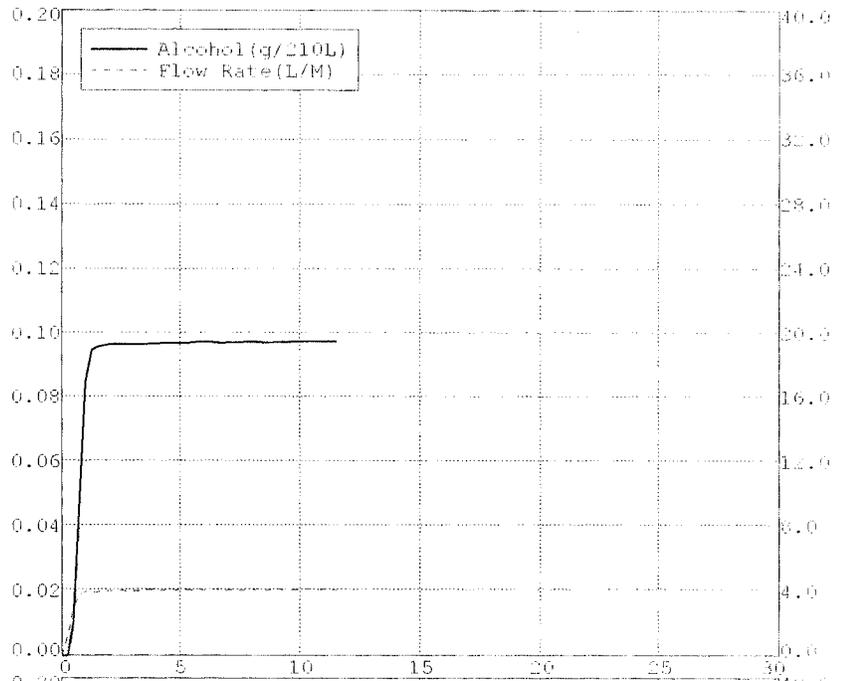

SUPERVISOR TEST




LAKE GEORGE
PARK COMMISSION
DATAMASTER dmt: 300391

Date: 06/22/2024

OPERATOR NAME:
JEFFREY W WEBSTER
Permit #: 13529
Operator Agency/Dept: LAKE GEORGE PK COMM
Reference Standard #: 24140

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:37
INTERNAL STANDARD	VERIFIED	10:37
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:38
BLANK TEST	0.00	10:39
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:39
BLANK TEST	0.00	10:40
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:40
BLANK TEST	0.00	10:41

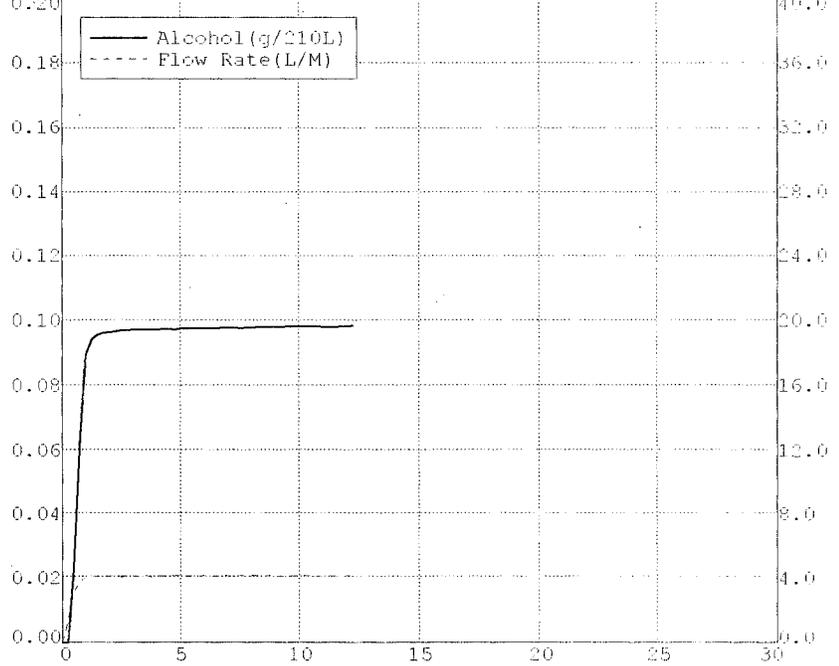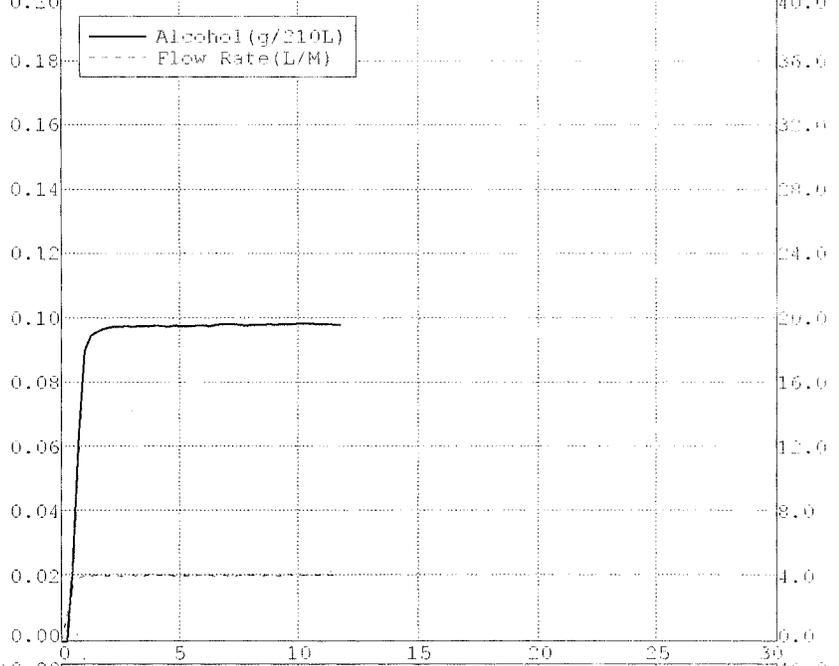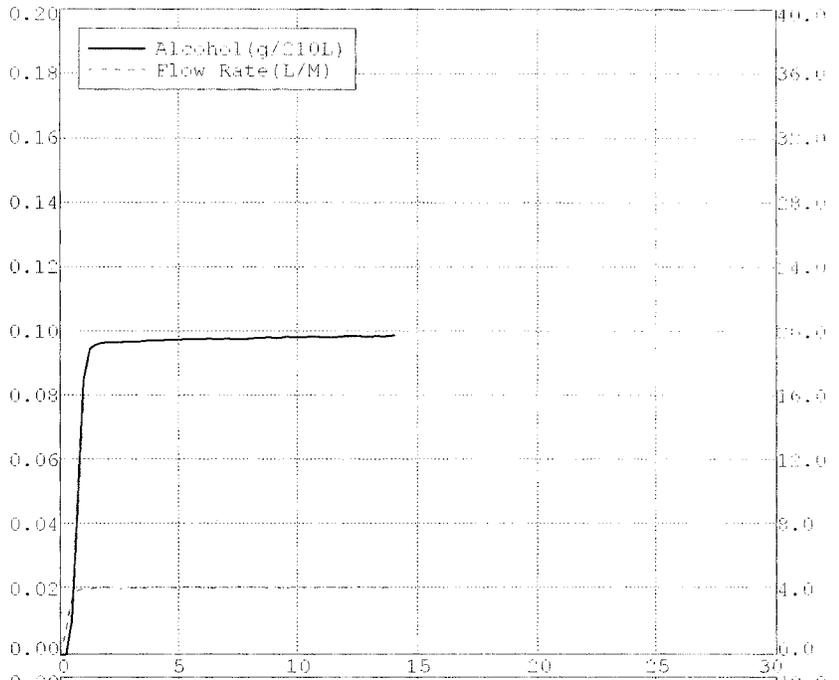

SUPERVISOR TEST




LAKE GEORGE
PARK COMMISSION
DATAMASTER dmt: 300391

Date: 06/17/2024

OPERATOR NAME:
ANGELO P PACCIONE
Permit #: 47655
Operator Agency/Dept: LAKE GEORGE PK COMM
Reference Standard #: 24140

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:25
INTERNAL STANDARD	VERIFIED	09:25
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	09:25
BLANK TEST	0.00	09:26
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	09:26
BLANK TEST	0.00	09:27
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	09:28
BLANK TEST	0.00	09:28

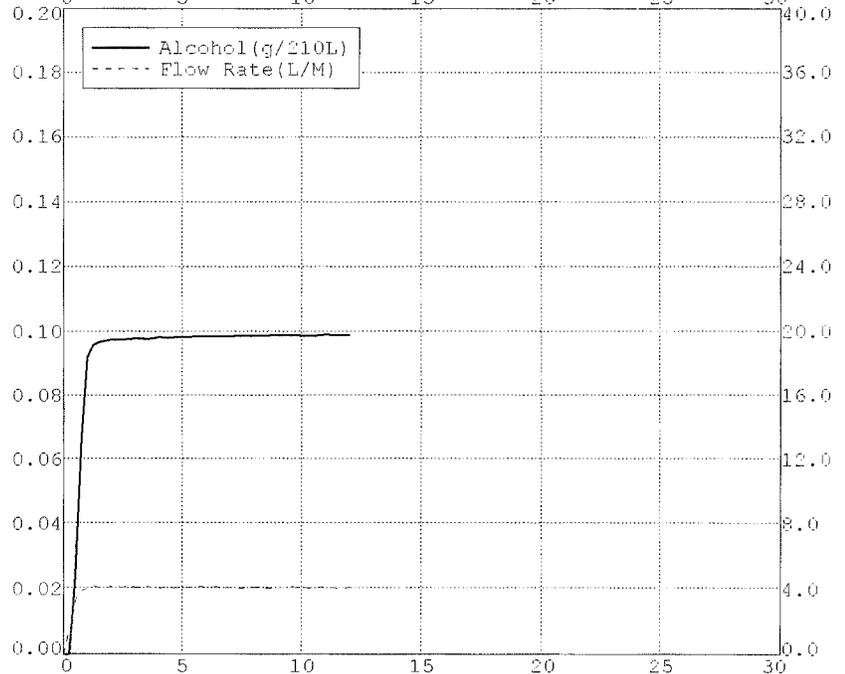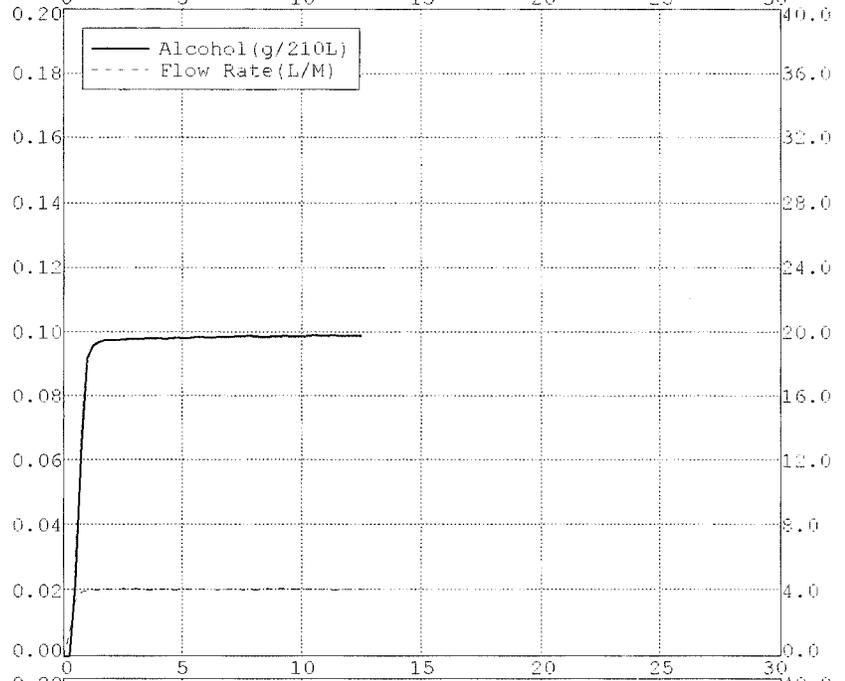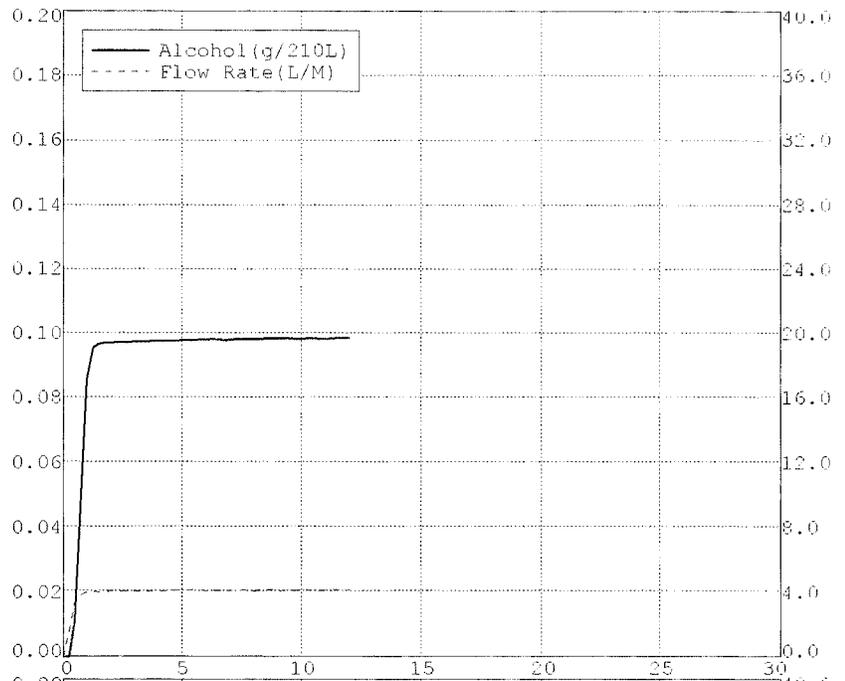

SUPERVISOR TEST




LAKE GEORGE
PARK COMMISSION
DATAMASTER dmt: 300391

Date: 06/08/2024

OPERATOR NAME:
JEFFREY W WEBSTER
Permit #: 13529
Operator Agency/Dept: LAKE GEORGE PK COMM
Reference Standard #: 24140

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:10
INTERNAL STANDARD	VERIFIED	10:10
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:10
BLANK TEST	0.00	10:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:12
BLANK TEST	0.00	10:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:13
BLANK TEST	0.00	10:14

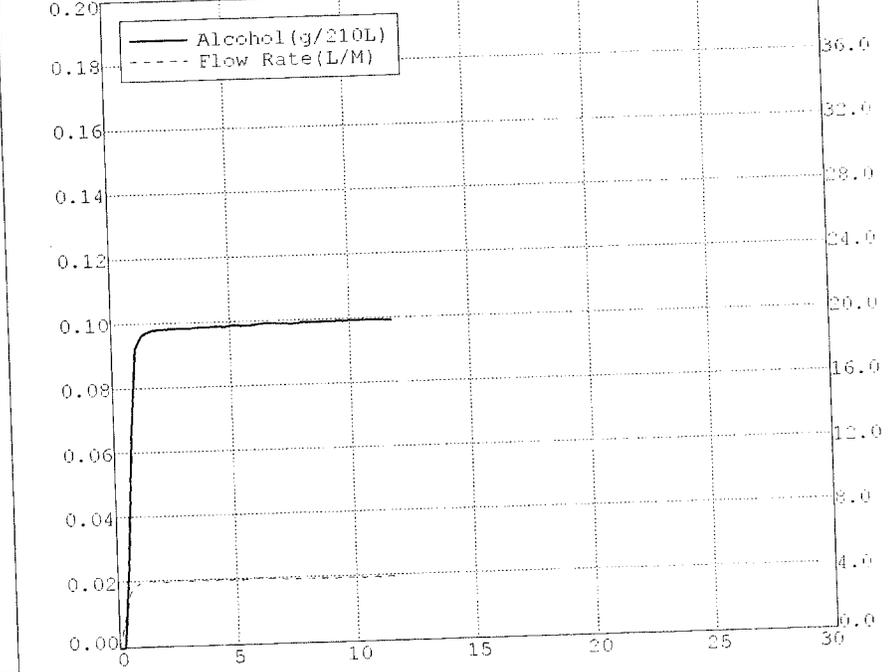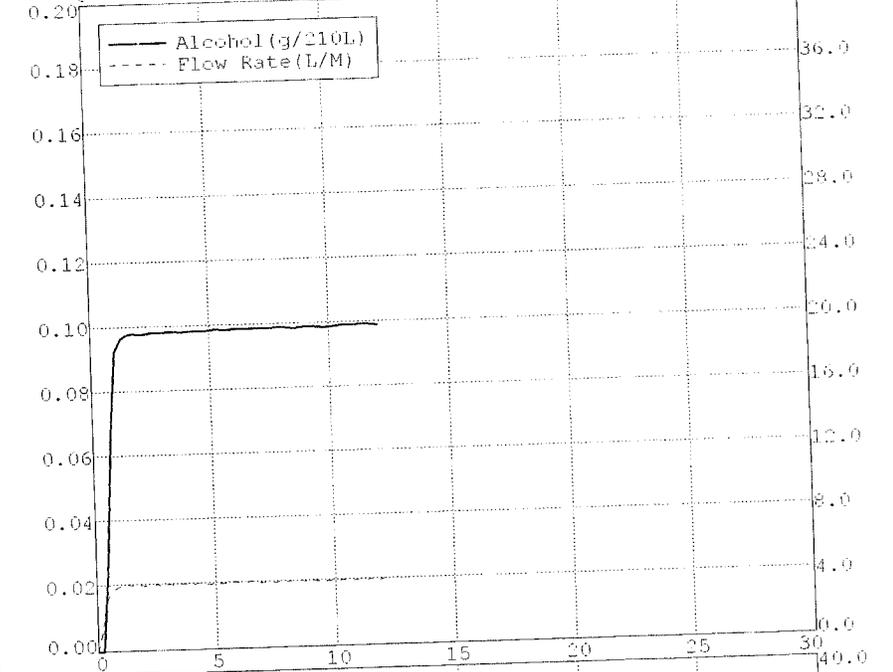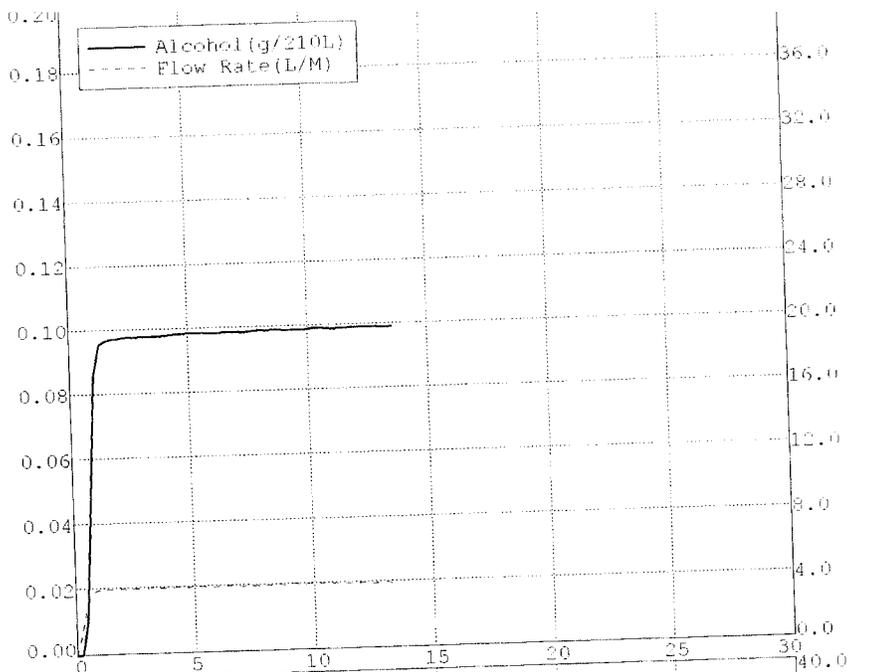

SOLUTION CHANGE




LAKE GEORGE
 PARK COMMISSION
 DATAMASTER dmt: 300391

Date: 06/01/2024

OPERATOR NAME:
 ANGELO P PACCIONE
 Permit #: 47655
 Operator Agency/Dept: LAKE GEORGE PK COMM
 Reference Standard #: 24140

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:38
INTERNAL STANDARD	34.01c	10:38
REFERENCE STANDARD TEMP	0.10	10:39
REFERENCE STANDARD	0.00	10:40
BLANK TEST	34.01c	10:40
REFERENCE STANDARD TEMP	0.09	10:40
REFERENCE STANDARD	0.00	10:41
BLANK TEST	34.01c	10:41
REFERENCE STANDARD TEMP	0.10	10:41
REFERENCE STANDARD	0.00	10:42
BLANK TEST		

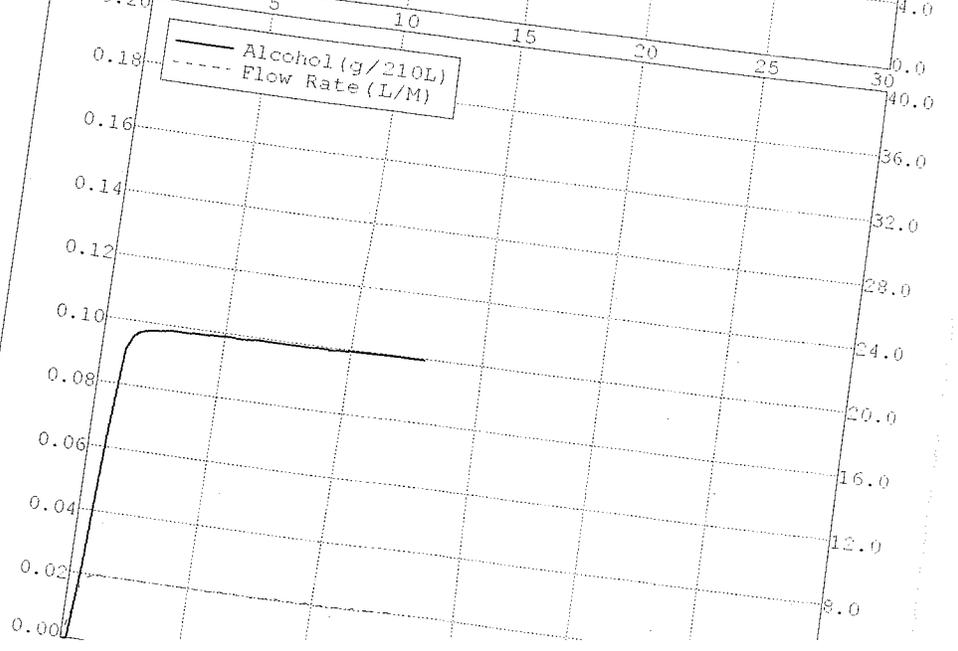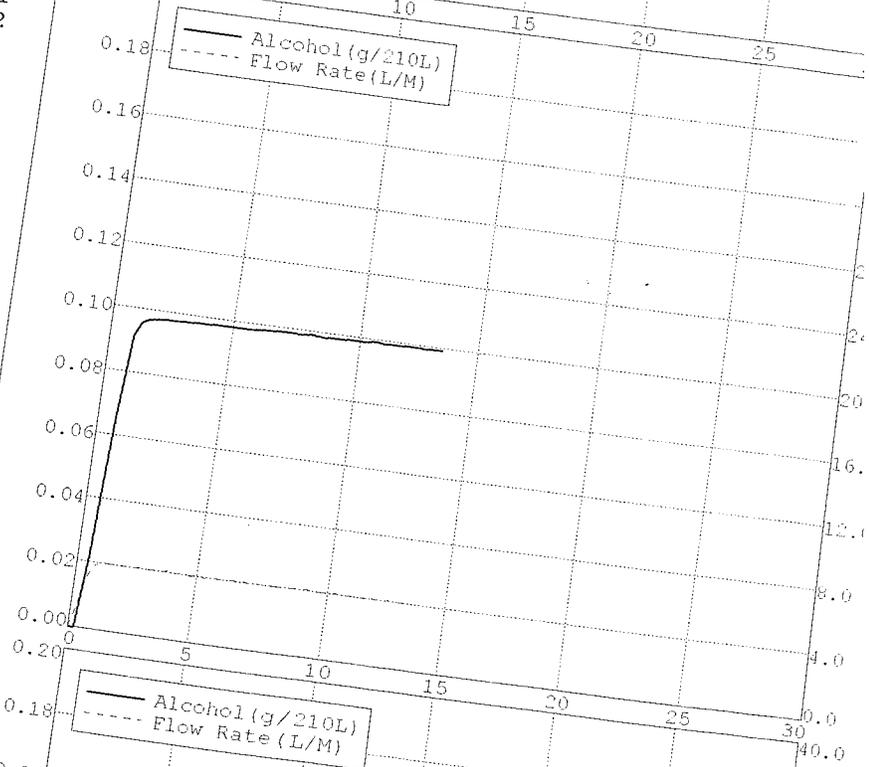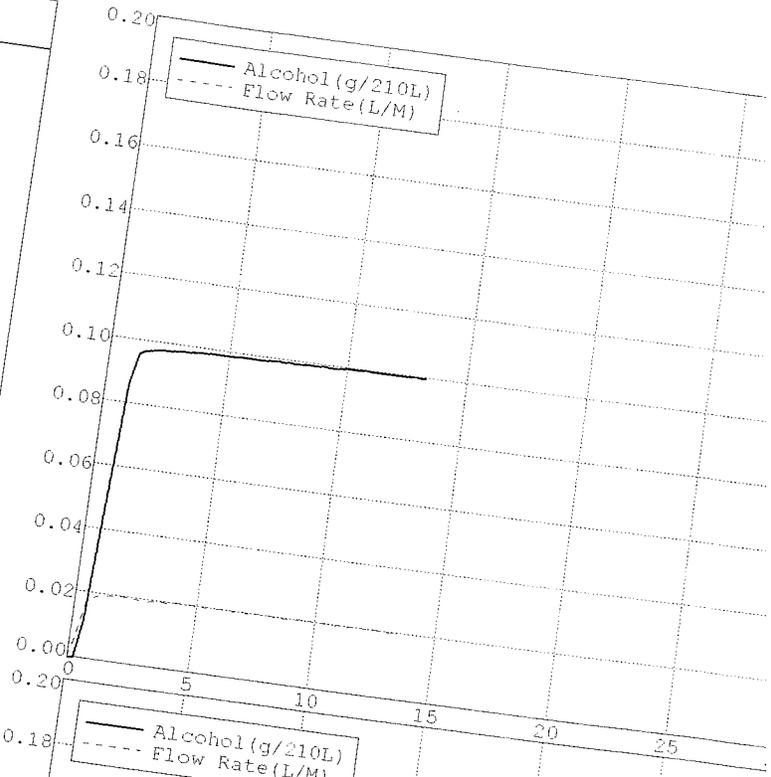

SUPERVISOR TEST




LAKE GEORGE
PARK COMMISSION
DATAMASTER dmt: 300391

Date: 05/25/2024

OPERATOR NAME:
JEFFREY W WEBSTER
Permit #: 13529
Operator Agency/Dept: LAKE GEORGE PK COMM
Reference Standard #: 24040

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:06
INTERNAL STANDARD	VERIFIED	09:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:06
BLANK TEST	0.00	09:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:07
BLANK TEST	0.00	09:08
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:09
BLANK TEST	0.00	09:09

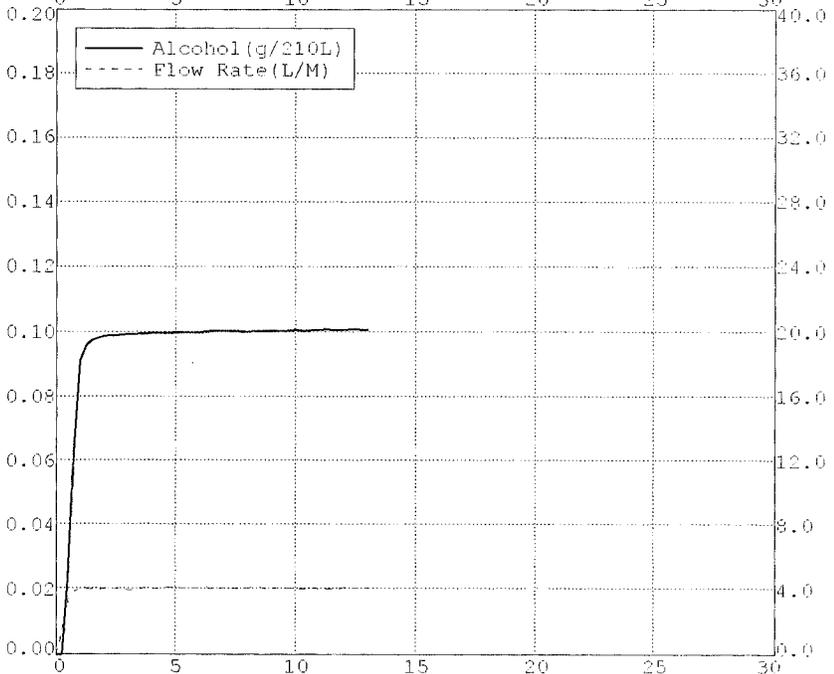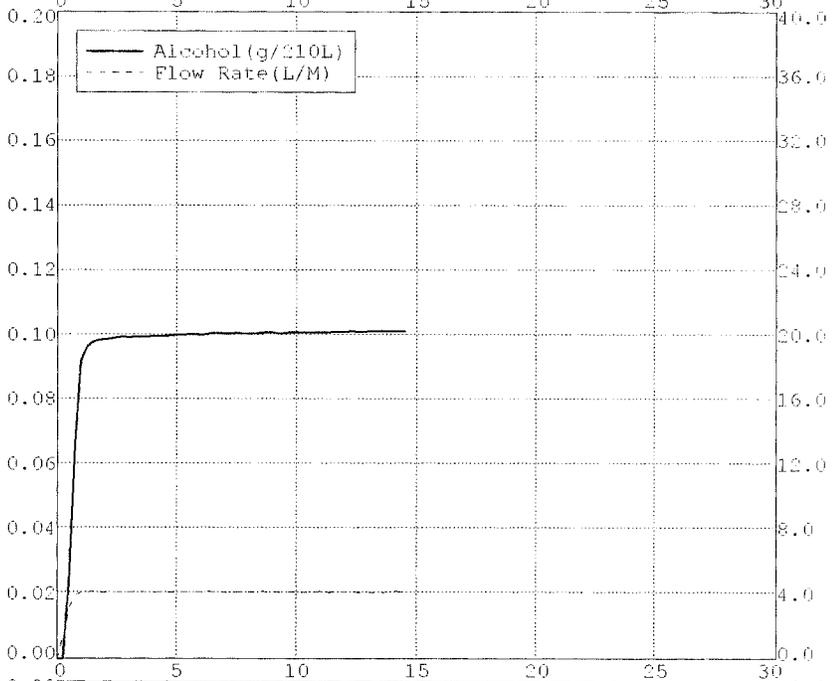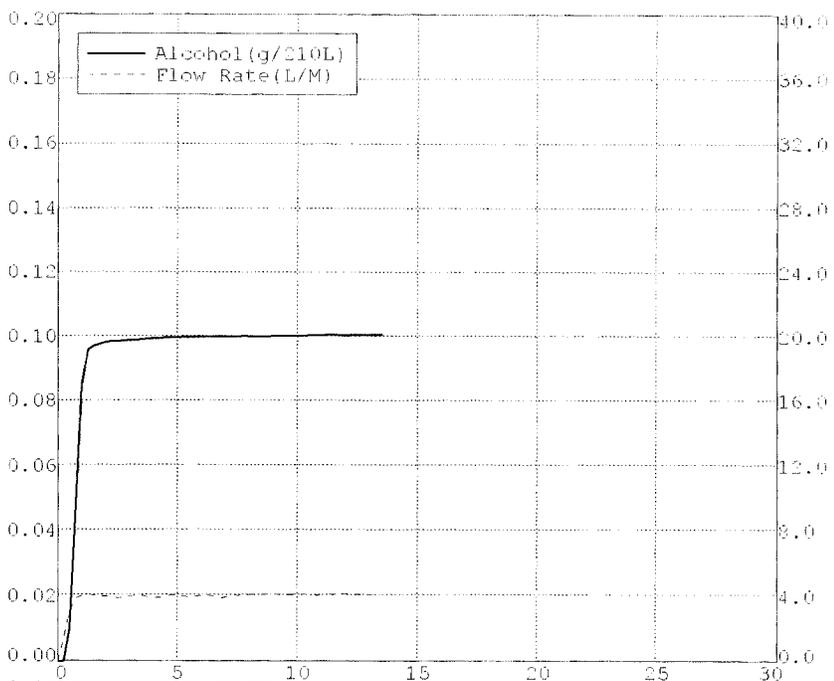

SOLUTION CHANGE

LAKE GEORGE
 PARK COMMISSION
 DATAMASTER dmt: 300391

Date: 05/18/2024

OPERATOR NAME:
 JEFFREY W WEBSTER
 Permit #: 13529
 Operator Agency/Dept: LAKE GEORGE PK COMM
 Reference Standard #: 24040

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:53
INTERNAL STANDARD	VERIFIED	09:53
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:53
BLANK TEST	0.00	09:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:54
BLANK TEST	0.00	09:55
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:55
BLANK TEST	0.00	09:56

