



## Division of Criminal Justice Services

---

### **CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS MAINTAINED IN THE REGULAR COURSE OF BUSINESS**

I, Joshua Vinehout, Supervisor of Public Safety Programs, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NAT'L PATENT ANALYTICAL SYS, DATAMASTER DMT breath test instrument, serial number 300391, performed on October 29, 2021 by Office of Public Safety employee Martin Schilling, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/ maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance /calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink that reads "Joshua Vinehout".

Digitally signed under  
ESRA by Joshua Vinehout  
on 11/4/2021 8:37 AM

---

**Joshua Vinehout**  
Supervisor of Public Safety Programs  
Office of Public Safety

An Equal Opportunity/Affirmative Action Agency

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Lake George Park Commission

Manufacturer: NAT'L PATENT ANALYTICAL SYS

Model: DATAMASTER DMT

Date: October 29, 2021

Serial Number: 300391

Reference Solution Lot Number: 21200

Reference Solution Standard: 0.10 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.100 %	34.01 degrees centigrade
2	0.099 %	34.01 degrees centigrade
3	0.099 %	34.01 degrees centigrade
4	0.099 %	34.01 degrees centigrade

Reference Solution Lot Number: 21310

Reference Solution Standard: 0.08 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.081 %	34.00 degrees centigrade
2	0.081 %	34.00 degrees centigrade
3	0.081 %	34.01 degrees centigrade
4	0.081 %	34.00 degrees centigrade

Reference Solution Lot Number: 21130

Reference Solution Standard: 0.180 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.180 %	34.01 degrees centigrade
2	0.180 %	34.01 degrees centigrade
3	0.180 %	34.01 degrees centigrade
4	0.180 %	34.00 degrees centigrade

I hereby certify that I have performed any necessary maintenance procedures and calibrated NAT'L PATENT ANALYTICAL SYS breath test instrument model DATAMASTER DMT, serial number 300391, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.

I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.

Performed by:



Digitally signed under  
ESRA by Martin Schilling  
on 10/29/2021 8:52 AM

**Martin Schilling**  
Highway Safety Equipment Technician  
Breath Analysis Operator Permit # 45926

Reviewed by:



Digitally signed under  
ESRA by Frank Sgarlata  
on 11/3/2021 10:17 AM

**Frank Sgarlata**  
Breath Analysis Technical Supervisor

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

**Name of Submitting Agency: Lake George Park Commission**  
**Manufacturer: NAT'L PATENT ANALYTICAL SYS**  
**Model: DATAMASTER DMT**  
**Serial Number: 300391**  
**Date: October 29, 2021**

- 1. General Appearance and condition of this device -----: OK**
  
- 2. Check controls and indicators -----: OK**
  
- 3. Check breath flow system -----: OK**
  
- 4. Check printer operation -----: OK**
  
- 5. System cycles through all modes -----: OK**



**6. Record any repairs made to this instrument and list services provided: INSPECTED INSTRUMENT, CHECKED SETUP VOLTAGES PRINT AND REMOTE OPERATION. RAN SUBJECT, TECHNICIAN AND DIAGNOSTIC TESTS, VERIFIED CALIBRATION.**

Performed by:

Digitally signed under  
ESRA by Martin Schilling  
on 10/29/2021 8:52 AM

---

**Martin Schilling**  
**Highway Safety Equipment Technician**  
**Breath Analysis Operator Permit # 45926**

Reviewed by:

Digitally signed under  
ESRA by Frank Sgarlata  
on 11/3/2021 10:17 AM

---

**Frank Sgarlata**  
**Breath Analysis Technical Supervisor**

TECHNICIAN TEST

LAKE GEORGE  
 PARK COMMISSION  
 DATAMASTER dmt: 300391





Date: 10/29/2021

OPERATOR NAME:  
 MARTIN J SCHILLING  
 Permit #: 45926  
 Operator Agency/Dept: LAKE GEORGE PK COMM  
 Reference Standard #: 21200

Nominal = 0.100 g/210L

BLANK TEST	0.000	07:38
INTERNAL STANDARD	VERIFIED	07:39
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.100	07:39
BLANK TEST	0.000	07:40
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.099	07:40
BLANK TEST	0.000	07:41
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.099	07:41
BLANK TEST	0.000	07:42
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.099	07:43
BLANK TEST	0.000	07:44

Average = 0.0992  
 Std Dev = 0.0005

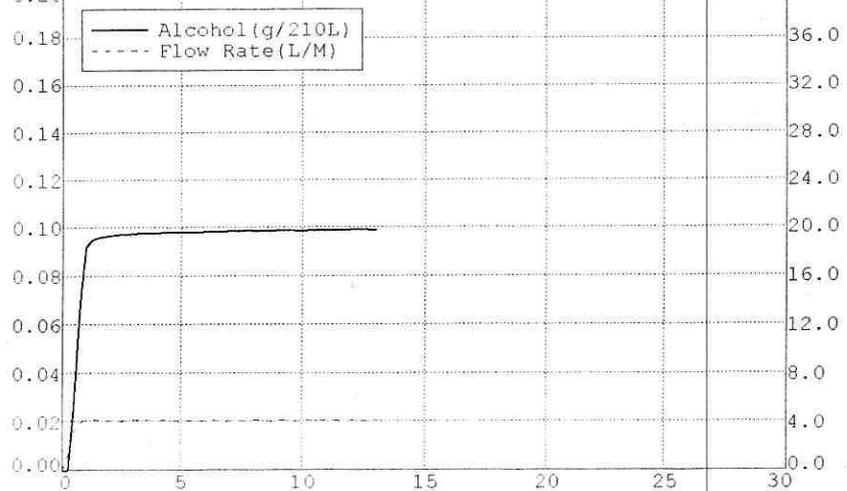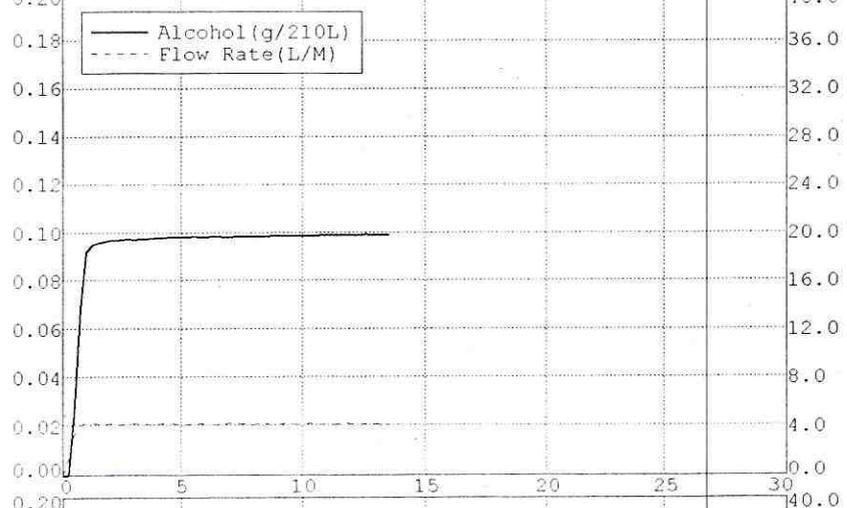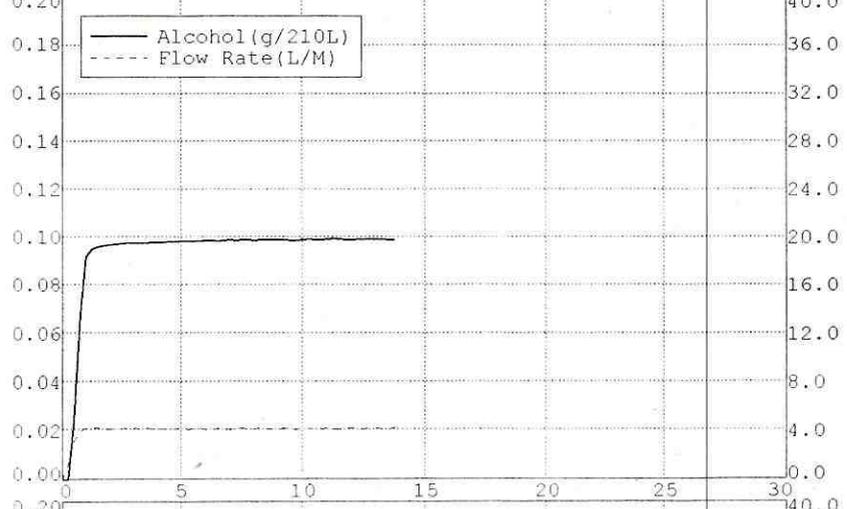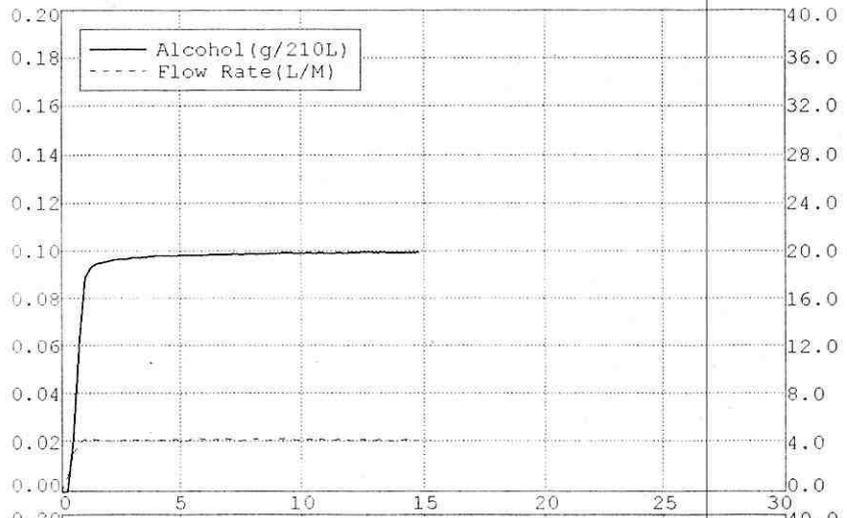

TECHNICIAN TEST

LAKE GEORGE  
 PARK COMMISSION  
 DATAMASTER dmt: 300391





Date: 10/29/2021

OPERATOR NAME:  
 MARTIN J SCHILLING  
 Permit #: 45926  
 Operator Agency/Dept: LAKE GEORGE PK COMM  
 Reference Standard #: 21310

Nominal = 0.080 g/210L

BLANK TEST	0.000	07:47
INTERNAL STANDARD	VERIFIED	07:47
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.081	07:47
BLANK TEST	0.000	07:48
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.081	07:49
BLANK TEST	0.000	07:49
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.081	07:50
BLANK TEST	0.000	07:51
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.081	07:51
BLANK TEST	0.000	07:52

Average = 0.0810  
 Std Dev = 0.0000

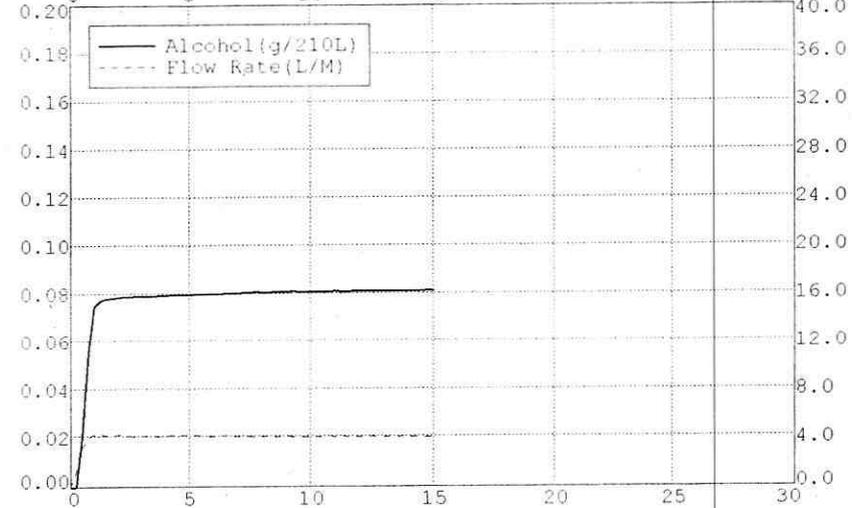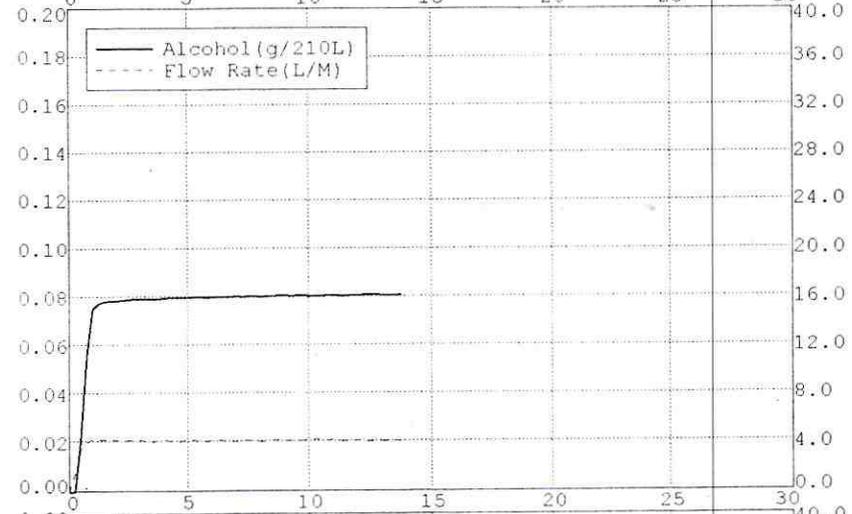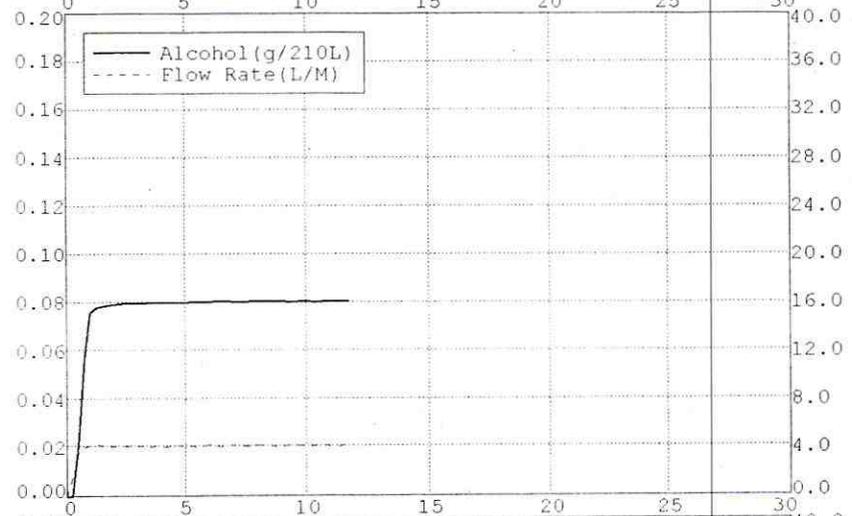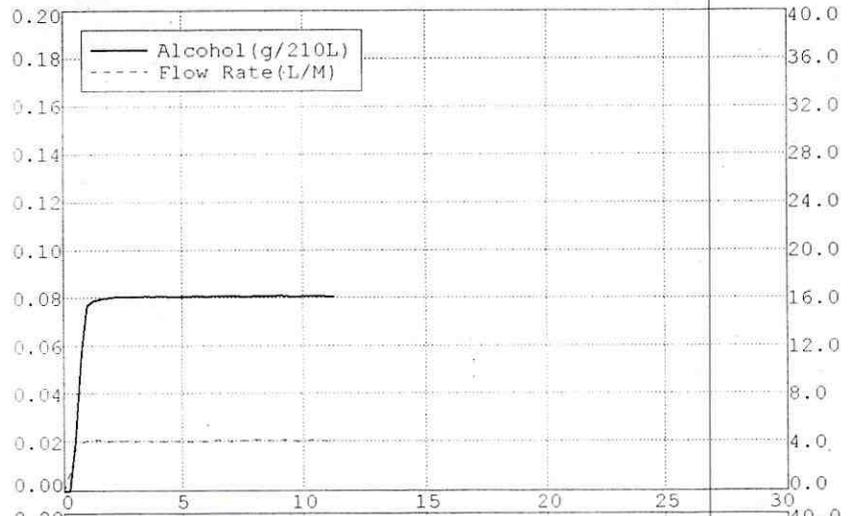

TECHNICIAN TEST

LAKE GEORGE  
 PARK COMMISSION  
 DATAMASTER dmt: 300391





Date: 10/29/2021

OPERATOR NAME:  
 MARTIN J SCHILLING  
 Permit #: 45926  
 Operator Agency/Dept: LAKE GEORGE PK COMM  
 Reference Standard #: 21130

Nominal = 0.180 g/210L

BLANK TEST	0.000	07:55
INTERNAL STANDARD	VERIFIED	07:55
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.180	07:55
BLANK TEST	0.000	07:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.180	07:57
BLANK TEST	0.000	07:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.180	07:58
BLANK TEST	0.000	07:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.180	07:59
BLANK TEST	0.000	08:00

Average = 0.1800  
 Std Dev = 0.0000

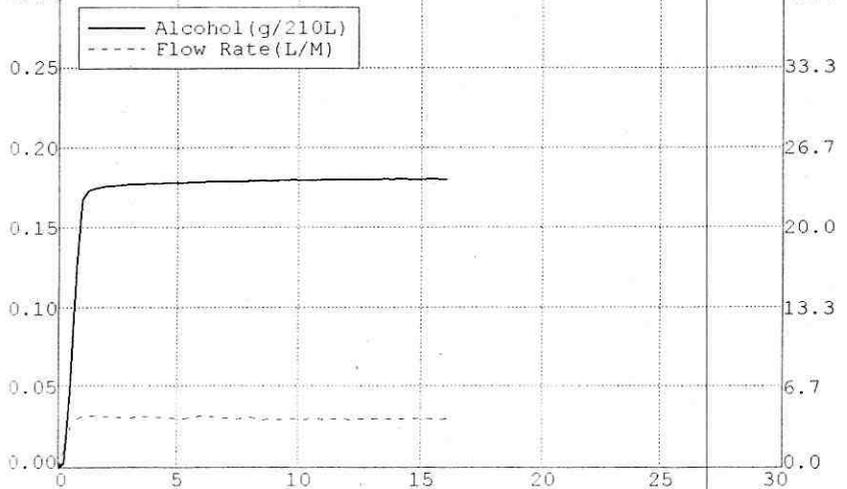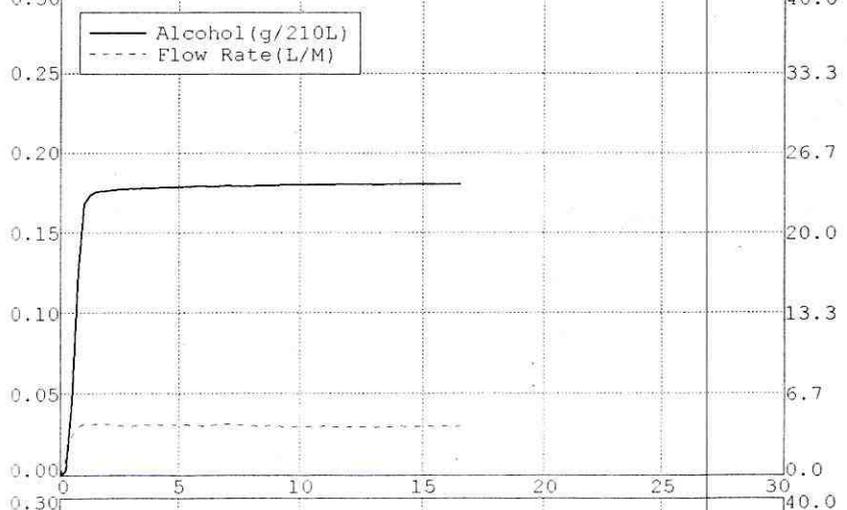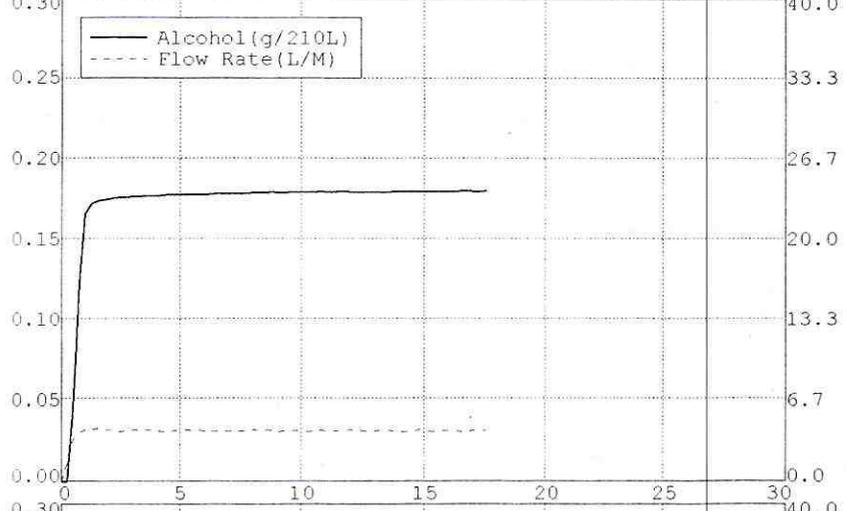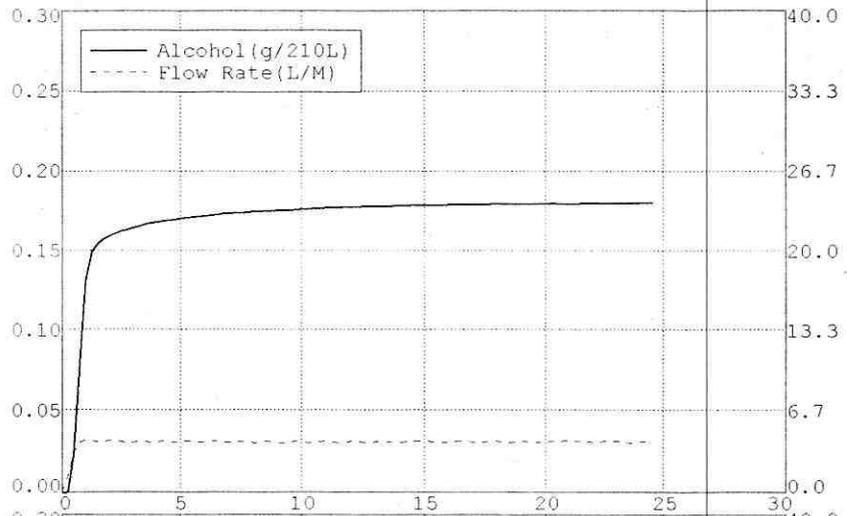

**SERVICE AUTHORIZATION FORM**  
**Highway Safety Technology Unit**  
 80 South Swan Street  
 Albany, NY 12210  
 Ph: 518-485-7636 / 518-402-0689  
 Fax: 518-457-6869

*NYJ*  
*10/29/21*

**THIS FORM IS USED TO AUTHORIZE THE DIVISION OF CRIMINAL JUSTICE SERVICES TO PERFORM SERVICE ON THE INSTRUMENT IDENTIFIED. THIS AUTHORIZATION MUST ACCOMPANY EACH PIECE OF EQUIPMENT WHEN IT IS PRESENTED TO THE EQUIPMENT REPAIR CENTER FOR SERVICE. PLEASE SIGN AND DATE FORM.**

**SECTION I - AGENCY INFORMATION**

Name of Agency <i>NYS Lake George Park Commission</i>		Today's Date <i>10/28/2021</i>
Address <i>75 Fort George Rd. P.O. Box 749</i>		City, State, ZIP <i>Lake George, NY 12845</i>
Contact Person <i>Lt. Joe Johns</i>		Contact Telephone <i>518-668-9347</i>
Contact Email <i>jjohns@lspc.state.ny.us</i>		Best Way to Reach You During Appointment Period <i>email</i>

**SECTION II - INSTRUMENT INFORMATION**

Instrument Manufacturer (Please Circle) <b>NPAS DMT</b> GUTH Applied Concepts(Stalker) Decatur(Genesis) Kustom(Eagle/Falcon) MPH Alco-Sensor Other:		
Model Number	Instrument Serial Number <i>300391</i>	
Antenna Serial Number (if applicable) Antenna 1 - / Antenna 2 -	Type of maintenance (check appropriate) <input checked="" type="checkbox"/> Calibration Check <input type="checkbox"/> Repair	
Brief Description of Malfunction <i>Drop off for Annual Check - will pick up in the Spring</i>		
List all parts, cables and/or accessories being submitted. <b>Tuning forks must accompany all radar units (if applicable).</b> (Please Circle)		
DMT/SIM: DMT            SIM            Tubes Keyboard      Other:	Radar: Control Unit      Antenna(s)      Antenna Cable(s) Power Cord      Forks            Other:	
<i>I acknowledge I am signing this Service Authorization Form as an act and deed of said agency, organization, or municipality, and that I am duly authorized to sign same for the uses and purposes mentioned herein. PLEASE SIGN AND DATE.</i>		
Signature <i>Lt. Joe Johns</i>	Date <i>10/28/2021</i>	

**DCJS USE ONLY**

*I inspected instrument. Checked setup and target point and remote operation. Ran software, technician and diagnostic tests. Verified calibration.*