



**CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS  
MAINTAINED IN THE REGULAR COURSE OF BUSINESS**

I, **Steven J. Carluccio**, Highway Safety Equipment Technical Supervisor, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NATL PATENT ANALYTICAL SYSTEM, DATAMASTER DMT breath test instrument, serial number 300391, performed on July 22, 2022 by Office of Public Safety employee George Coffin, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance /calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink that reads "Steven J. Carluccio".

Digitally signed under ESRA  
by Steven J. Carluccio  
on 08/02/2022 07:42 AM

---

**Steven J. Carluccio**  
**Highway Safety Equipment Technical Supervisor**  
**Office of Public Safety**

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Lake George Park Commission

Manufacturer: NATL PATENT ANALYTICAL SYSTEM

Model: DATAMASTER DMT

Serial Number: 300391

Date: July 22, 2022

Reference Solution Lot Number : 22120

Reference Solution Standard : 0.10% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.099 %	34.01 degrees centigrade
2	0.099 %	34.01 degrees centigrade
3	0.099 %	34.01 degrees centigrade
4	0.099 %	34.01 degrees centigrade

Reference Solution Lot Number : 21310

Reference Solution Standard : 0.08% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.080 %	34.01 degrees centigrade
2	0.080 %	34.01 degrees centigrade
3	0.080 %	34.01 degrees centigrade
4	0.080 %	34.02 degrees centigrade

Reference Solution Lot Number : 22060

Reference Solution Standard : 0.18% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.179 %	34.01 degrees centigrade
2	0.179 %	34.01 degrees centigrade
3	0.180 %	34.01 degrees centigrade
4	0.180 %	34.01 degrees centigrade

I hereby certify that I have performed any necessary maintenance procedures and calibrated NATL PATENT ANALYTICAL SYSTEM breath test instrument model DATAMASTER DMT, serial number 300391, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.

I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.

Performed by:



Digitally signed under ESRA  
by George Coffin  
on 07/22/2022 02:11 PM

Reviewed by:



Digitally signed under ESRA  
by Frank Sgarlata  
on 07/22/2022 02:34 PM

**George Coffin**  
Highway Safety Equipment Technician  
Breath Analysis Operator Permit #48534

**Frank Sgarlata**  
Breath Analysis Technical Supervisor

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

**Name of Submitting Agency: Lake George Park Commission**

**Manufacturer: NATL PATENT ANALYTICAL SYSTEM**

**Model: DATAMASTER DMT**

**Serial Number: 300391**

**Date: July 22, 2022**

**1. General appearance and condition of this device -----: INTERFERENCE,  
SIM TIMEOUT ERRORS.**

**2. Check controls and indicators -----: OK**

**3. Check breath flow system -----: OK**

**4. Check printer operation -----: OK**

**5. System cycles through all modes -----: OK**



**6. Record any repairs made to this instrument and list services provided : CLEANED AND  
ADJUSTED FILTER WHEEL ASSEMBLY, REPLACED DETECTOR. INSPECTED  
INSTRUMENT, CHECKED SETUP VOLTAGES PRINT AND REMOTE OPERATION.  
PERFORMED CALIBRATION/ADJUSTMENT PROCEDURE, RAN SUBJECT,  
TECHNICIAN AND DIAGNOSTIC TESTS, VERIFIED CALIBRATION.**

Performed by:

Digitally signed under ESRA  
by George Coffin  
on 07/22/2022 02:11 PM

Reviewed by:

Digitally signed under ESRA  
by Frank Sgarlata  
on 07/22/2022 02:34 PM

---

**George Coffin  
Highway Safety Equipment Technician  
Breath Analysis Operator Permit #48534**

---

**Frank Sgarlata  
Breath Analysis Technical Supervisor**

TECHNICIAN TEST

LAKE GEORGE  
 PARK COMMISSION  
 DATAMASTER dmt: 300391





Date: 07/22/2022

OPERATOR NAME:  
 GEORGE R COFFIN  
 Permit #: 48534  
 Operator Agency/Dept: LAKE GEORGE PK COMM  
 Reference Standard #: 21310

Nominal = 0.080 g/210L

BLANK TEST	0.000	11:09
INTERNAL STANDARD	VERIFIED	11:09
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.080	11:09
BLANK TEST	0.000	11:10
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.080	11:10
BLANK TEST	0.000	11:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.080	11:12
BLANK TEST	0.000	11:12
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.080	11:13
BLANK TEST	0.000	11:14

Average = 0.0800  
 Std Dev = 0.0000

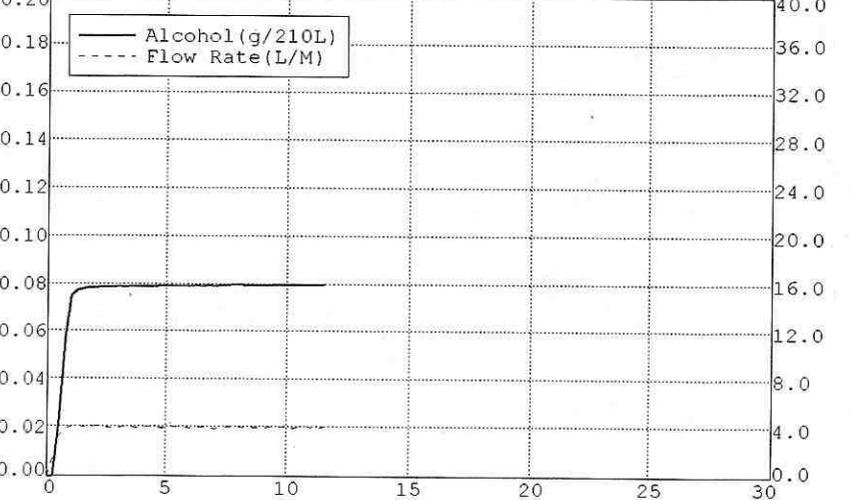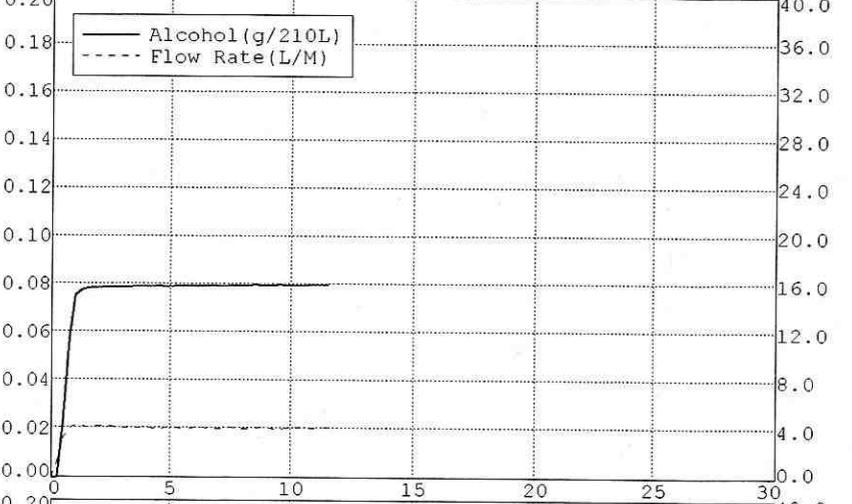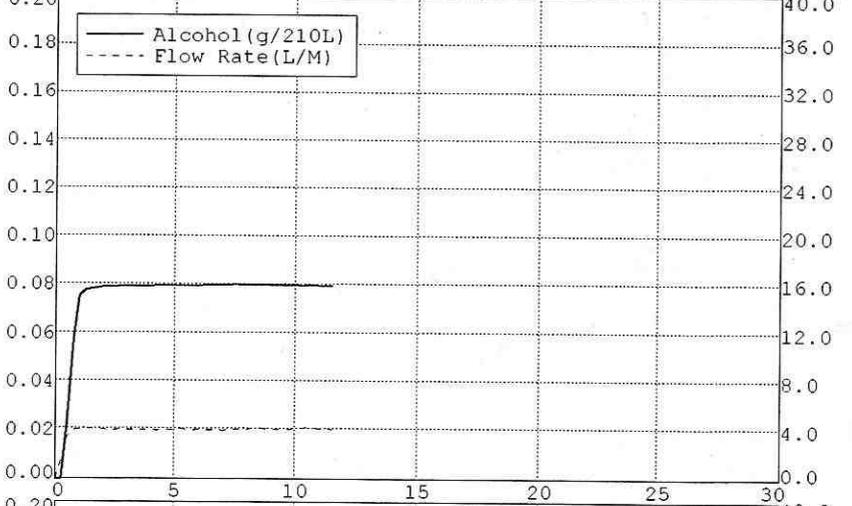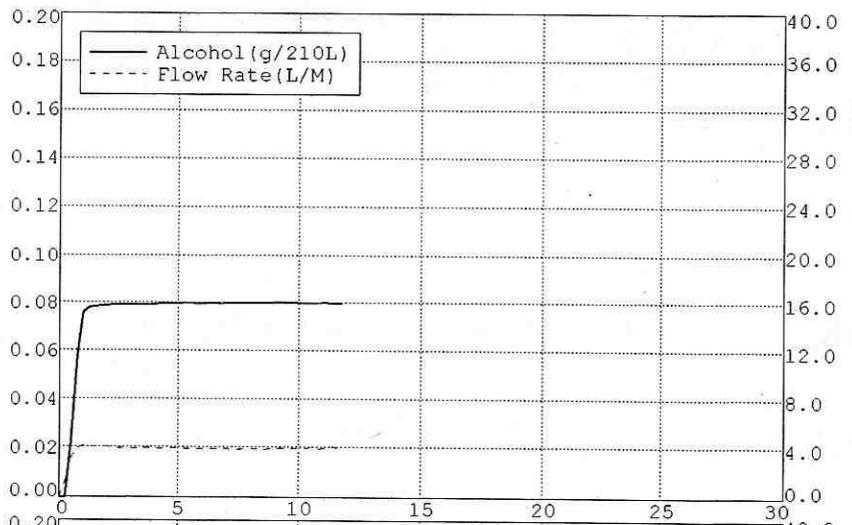

TECHNICIAN TEST

LAKE GEORGE  
 PARK COMMISSION  
 DATAMASTER dmt: 300391





Date: 07/22/2022

OPERATOR NAME:  
 GEORGE R COFFIN  
 Permit #: 48534  
 Operator Agency/Dept: LAKE GEORGE PK COMM  
 Reference Standard #: 22120

Nominal = 0.100 g/210L

BLANK TEST	0.000	11:17
INTERNAL STANDARD	VERIFIED	11:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.099	11:17
BLANK TEST	0.000	11:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.099	11:18
BLANK TEST	0.000	11:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.099	11:20
BLANK TEST	0.000	11:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.099	11:21
BLANK TEST	0.000	11:22

Average = 0.0990  
 Std Dev = 0.0000

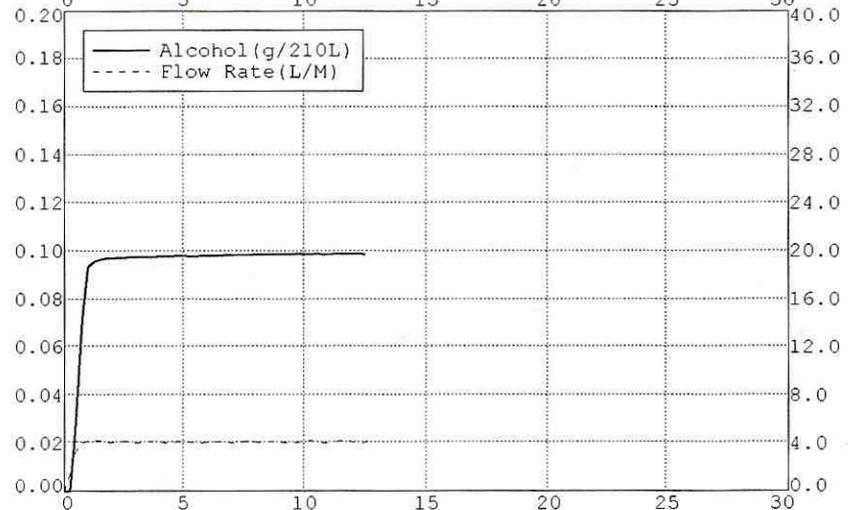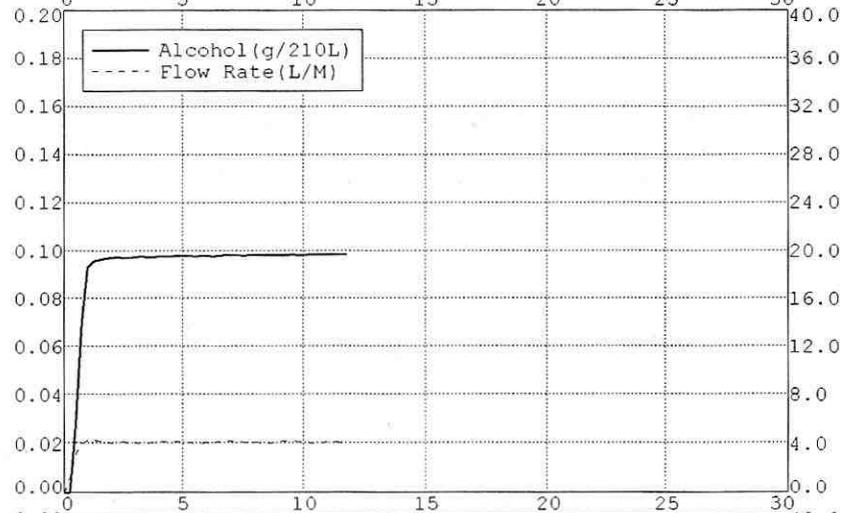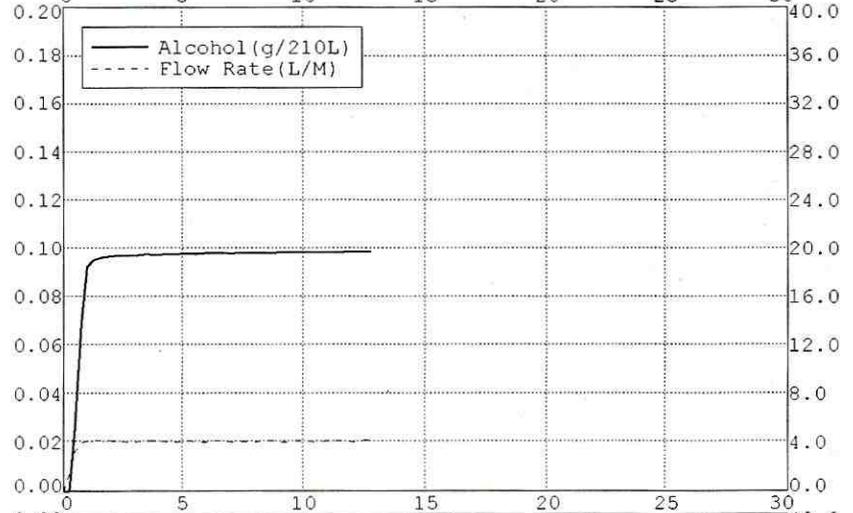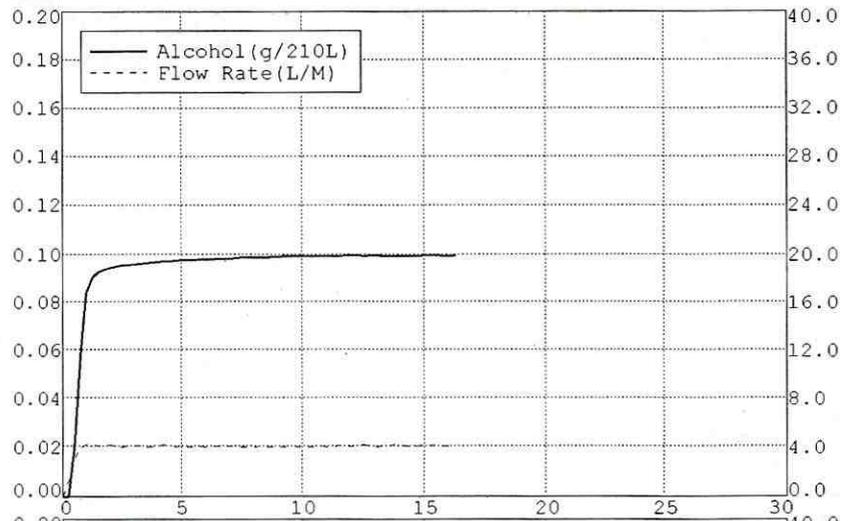

TECHNICIAN TEST

LAKE GEORGE  
PARK COMMISSION  
DATAMASTER dmt: 300391

Date: 07/22/2022

OPERATOR NAME:  
GEORGE R COFFIN  
Permit #: 48534  
Operator Agency/Dept: LAKE GEORGE PK COMM  
Reference Standard #: 22060

Nominal = 0.180 g/210L

BLANK TEST	0.000	11:33
INTERNAL STANDARD	VERIFIED	11:33
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.179	11:33
BLANK TEST	0.000	11:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.179	11:35
BLANK TEST	0.000	11:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.180	11:36
BLANK TEST	0.000	11:37
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.180	11:37
BLANK TEST	0.000	11:38

Average = 0.1795  
Std Dev = 0.0006

