



**CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS
MAINTAINED IN THE REGULAR COURSE OF BUSINESS**

I, Steven J. Carluccio, Highway Safety Equipment Technical Supervisor, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NATL PATENT ANALYTICAL SYSTEM, DATAMASTER DMT breath test instrument, serial number 300391, performed on May 02, 2023 by Office of Public Safety employee Martin Schilling, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance /calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink that reads "Steven J. Carluccio".

Digitally signed under ESRA
by Steven J. Carluccio
on 05/11/2023 10:16 AM

Steven J. Carluccio
Highway Safety Equipment Technical Supervisor
Office of Public Safety

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Lake George Park Commission

Manufacturer: NATL PATENT ANALYTICAL SYSTEM

Model: DATAMASTER DMT

Serial Number: 300391

Date: May 02, 2023

Reference Solution Lot Number : 23050

Reference Solution Standard : 0.10% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.100 %	34.02 degrees centigrade
2	0.100 %	34.02 degrees centigrade
3	0.100 %	34.02 degrees centigrade
4	0.101 %	34.02 degrees centigrade

Reference Solution Lot Number : 22210

Reference Solution Standard : 0.08% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.080 %	34.02 degrees centigrade
2	0.079 %	34.02 degrees centigrade
3	0.079 %	34.02 degrees centigrade
4	0.079 %	34.02 degrees centigrade

Reference Solution Lot Number : 22450

Reference Solution Standard : 0.18% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.179 %	34.02 degrees centigrade
2	0.180 %	34.02 degrees centigrade
3	0.180 %	34.02 degrees centigrade
4	0.180 %	34.02 degrees centigrade

I hereby certify that I have performed any necessary maintenance procedures and calibrated NATL PATENT ANALYTICAL SYSTEM breath test instrument model DATAMASTER DMT, serial number 300391, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.

I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.

Performed by:



Digitally signed under ESRA
by Martin Schilling
on 05/02/2023 01:14 PM

Reviewed by:



Digitally signed under ESRA
by Frank Sgarlata
on 05/02/2023 01:17 PM

Martin Schilling
Highway Safety Equipment Technician
Breath Analysis Operator Permit #45926

Frank Sgarlata
Breath Analysis Technical Supervisor

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Lake George Park Commission
Manufacturer: NATL PATENT ANALYTICAL SYSTEM
Model: DATAMASTER DMT
Serial Number: 300391
Date: May 02, 2023

- 1. General appearance and condition of this device -----: **OK**

- 2. Check controls and indicators -----: **OK**

- 3. Check breath flow system -----: **OK**

- 4. Check printer operation -----: **OK**

- 5. System cycles through all modes -----: **OK**



6. Record any repairs made to this instrument and list services provided : INSPECTED INSTRUMENT, CHECKED SETUP VOLTAGES PRINT AND REMOTE OPERATION. PERFORMED CALIBRATION/ADJUSTMENT PROCEDURE, RAN SUBJECT, TECHNICIAN AND DIAGNOSTIC TESTS, VERIFIED CALIBRATION.

Performed by:

Handwritten signature of Martin Schilling in black ink.

Digitally signed under ESRA
by Martin Schilling
on 05/02/2023 01:14 PM

Reviewed by:

Handwritten signature of Frank Sgarlata in black ink.

Digitally signed under ESRA
by Frank Sgarlata
on 05/02/2023 01:17 PM

Martin Schilling
Highway Safety Equipment Technician
Breath Analysis Operator Permit #45926

Frank Sgarlata
Breath Analysis Technical Supervisor

TECHNICIAN TEST

LAKE GEORGE
 PARK COMMISSION
 DATAMASTER dmt: 300391





Date: 05/02/2023

OPERATOR NAME:
 MARTIN J SCHILLING
 Permit #: 45926
 Operator Agency/Dept: LAKE GEORGE PK COMM
 Reference Standard #: 22210

Nominal = 0.080 g/210L

BLANK TEST	0.000	10:23
INTERNAL STANDARD	VERIFIED	10:23
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.080	10:24
BLANK TEST	0.000	10:24
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.079	10:25
BLANK TEST	0.000	10:26
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.079	10:26
BLANK TEST	0.000	10:27
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.079	10:27
BLANK TEST	0.000	10:28

Average = 0.0792
 Std Dev = 0.0005

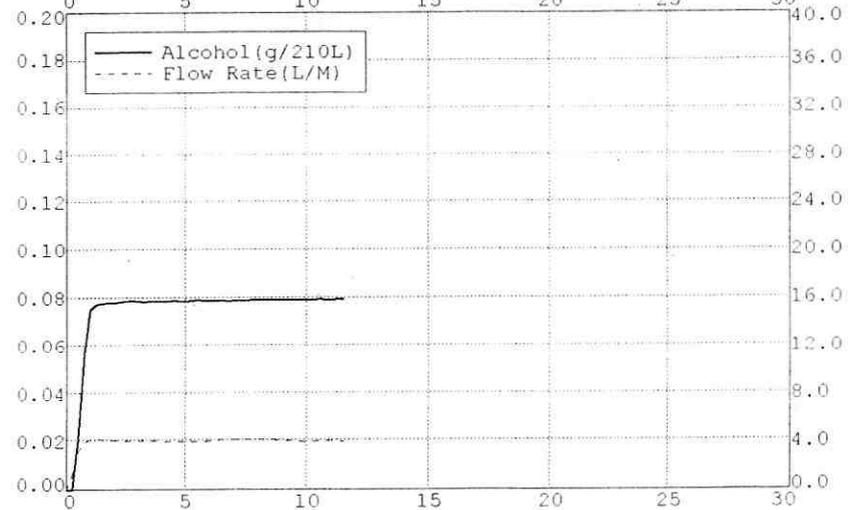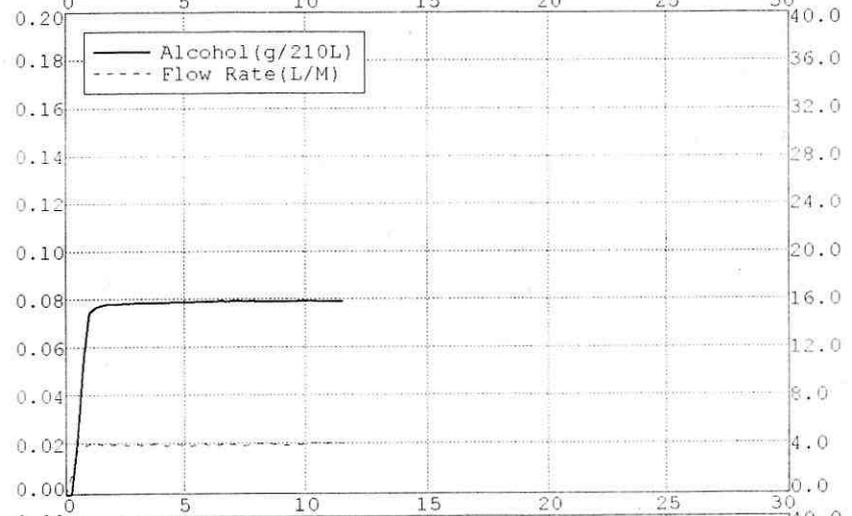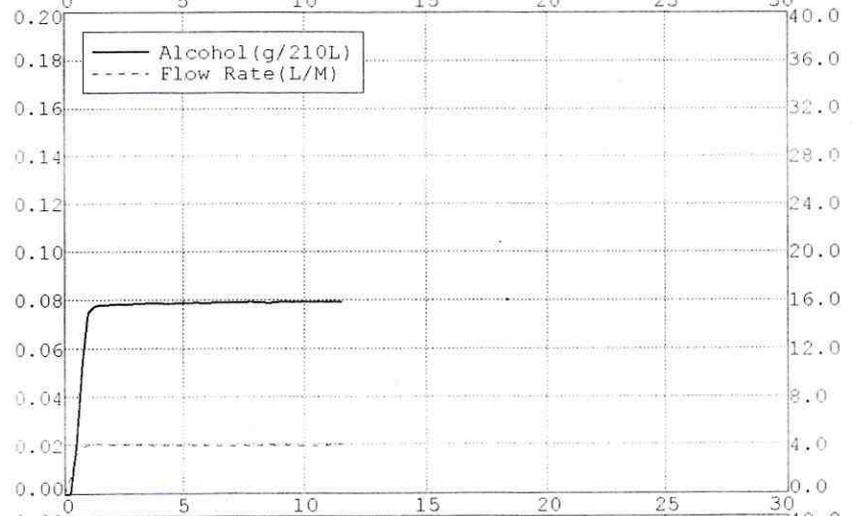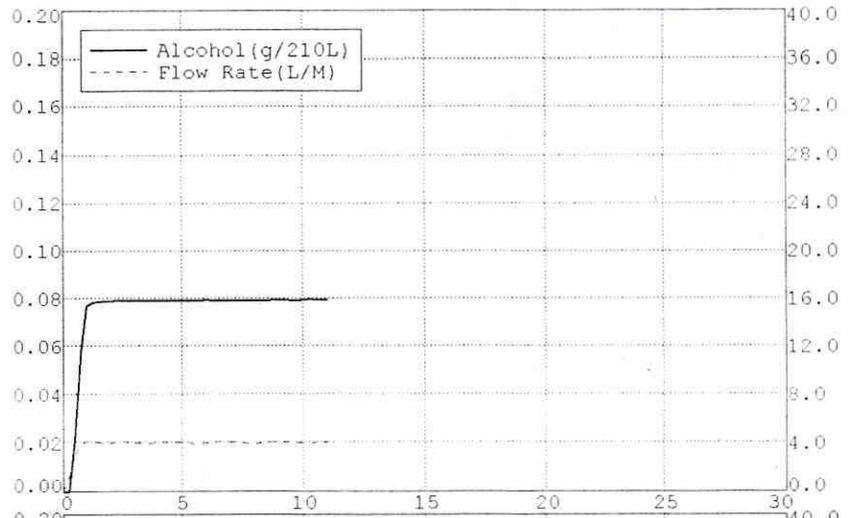

TECHNICIAN TEST

LAKE GEORGE
 PARK COMMISSION
 DATAMASTER dmt: 300391





Date: 05/02/2023

OPERATOR NAME:
 MARTIN J SCHILLING
 Permit #: 45926
 Operator Agency/Dept: LAKE GEORGE PK COMM
 Reference Standard #: 23050

Nominal = 0.100 g/210L

BLANK TEST	0.000	10:01
INTERNAL STANDARD	VERIFIED	10:01
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.100	10:01
BLANK TEST	0.000	10:02
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.100	10:02
BLANK TEST	0.000	10:03
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.100	10:03
BLANK TEST	0.000	10:04
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.101	10:05
BLANK TEST	0.000	10:06

Average = 0.1003
 Std Dev = 0.0005

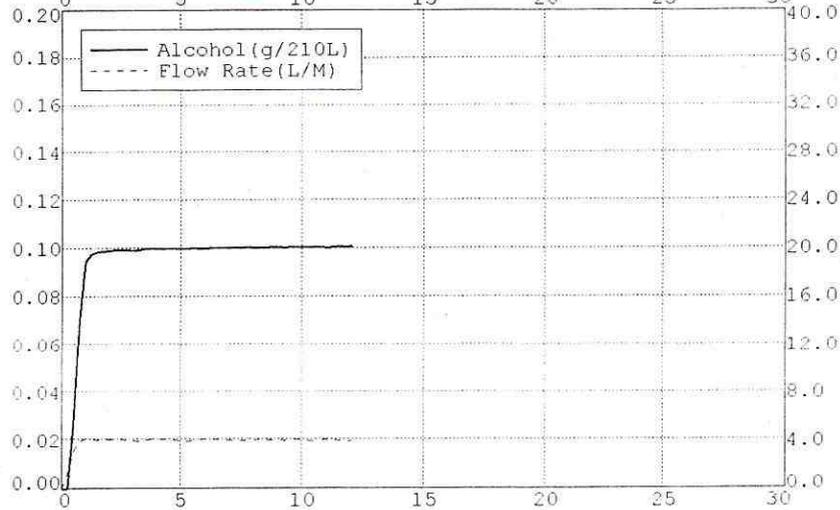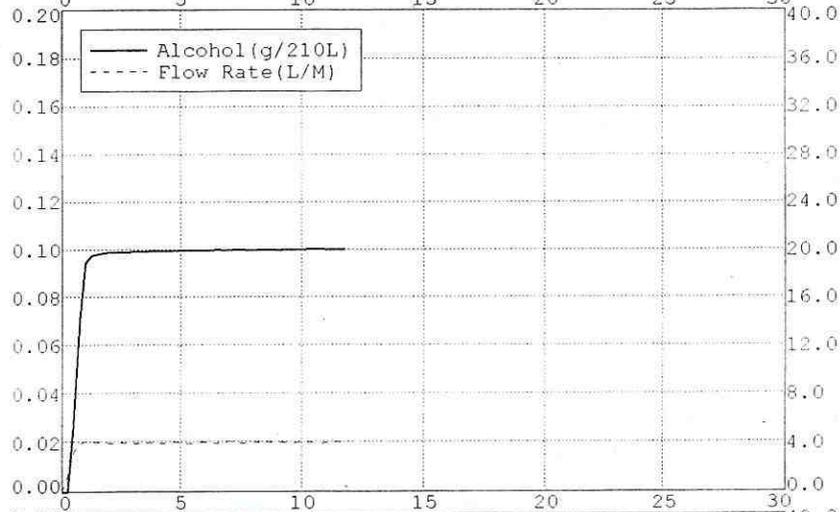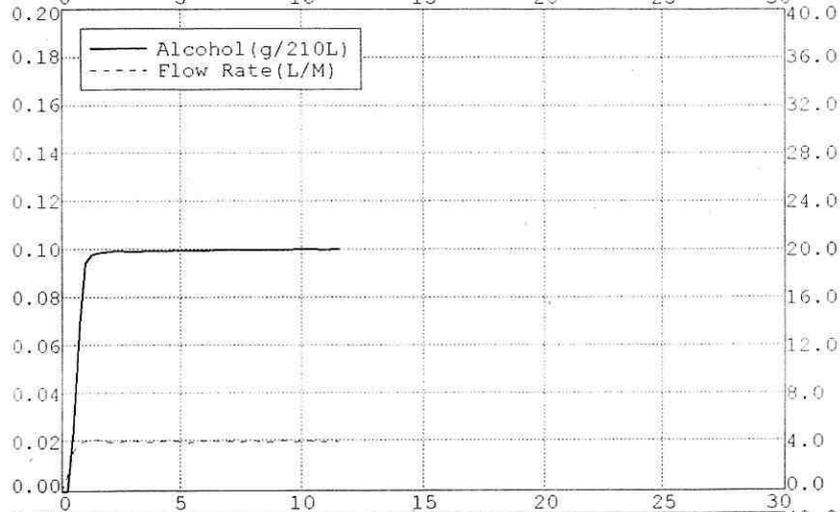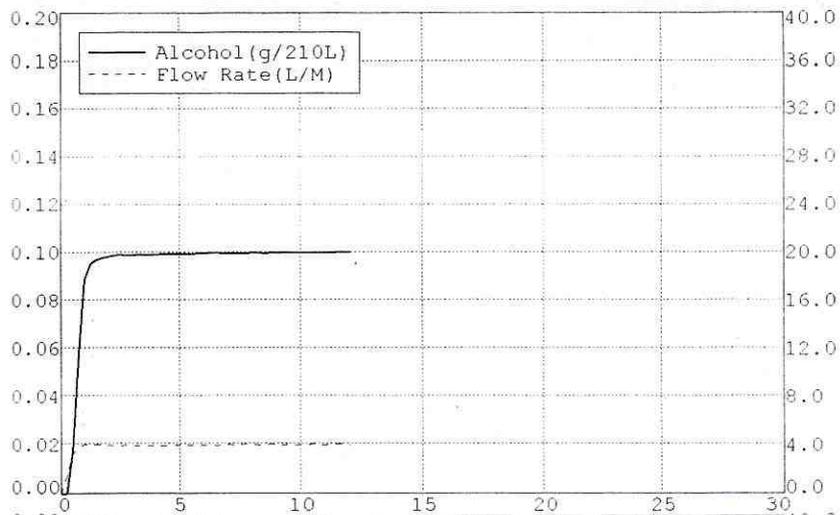

TECHNICIAN TEST

LAKE GEORGE
 PARK COMMISSION
 DATAMASTER dmt: 300391





Date: 05/02/2023

OPERATOR NAME:
 MARTIN J SCHILLING
 Permit #: 45926
 Operator Agency/Dept: LAKE GEORGE PK COMM
 Reference Standard #: 22450

Nominal = 0.180 g/210L

BLANK TEST	0.000	11:21
INTERNAL STANDARD	VERIFIED	11:21
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.179	11:21
BLANK TEST	0.000	11:22
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.180	11:23
BLANK TEST	0.000	11:23
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.180	11:24
BLANK TEST	0.000	11:25
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.180	11:25
BLANK TEST	0.000	11:26

Average = 0.1798
 Std Dev = 0.0005

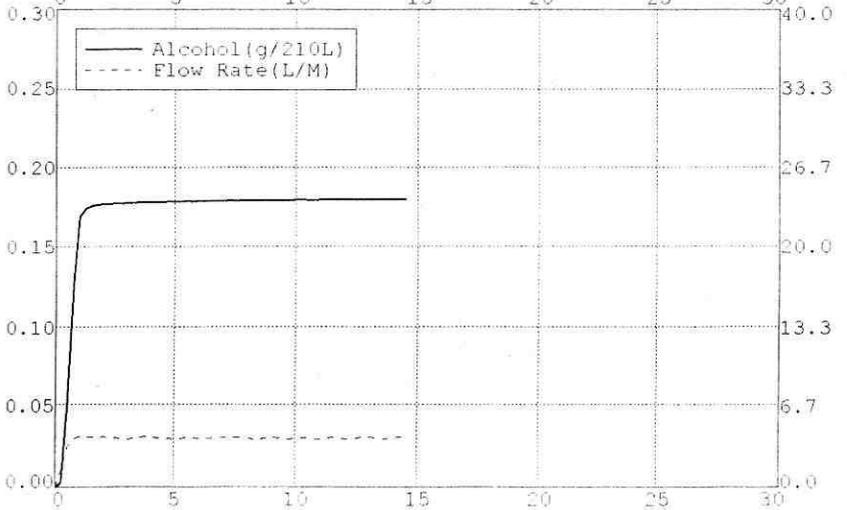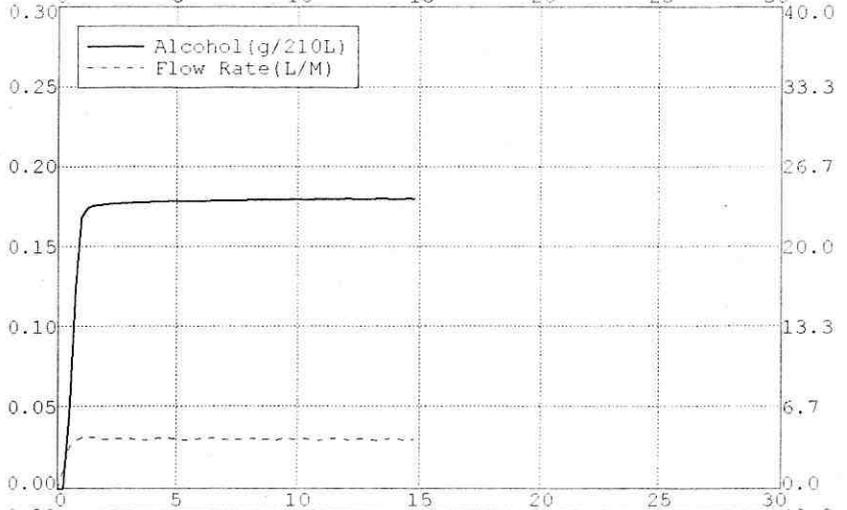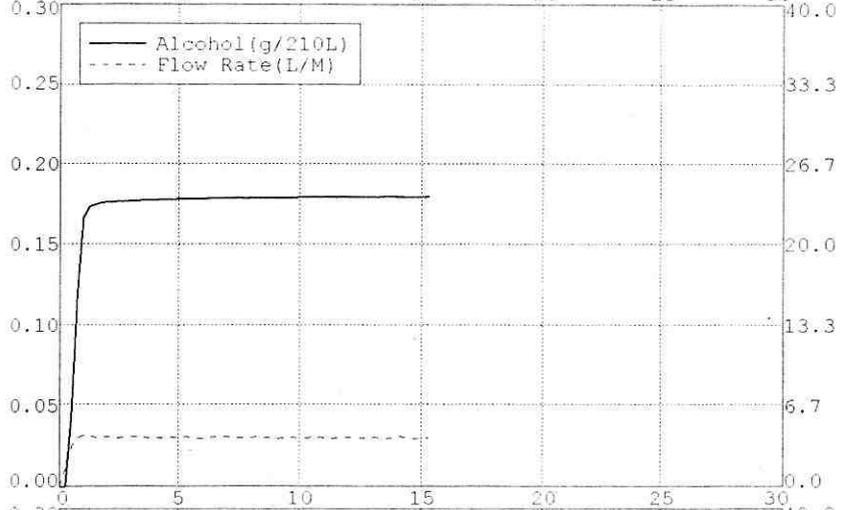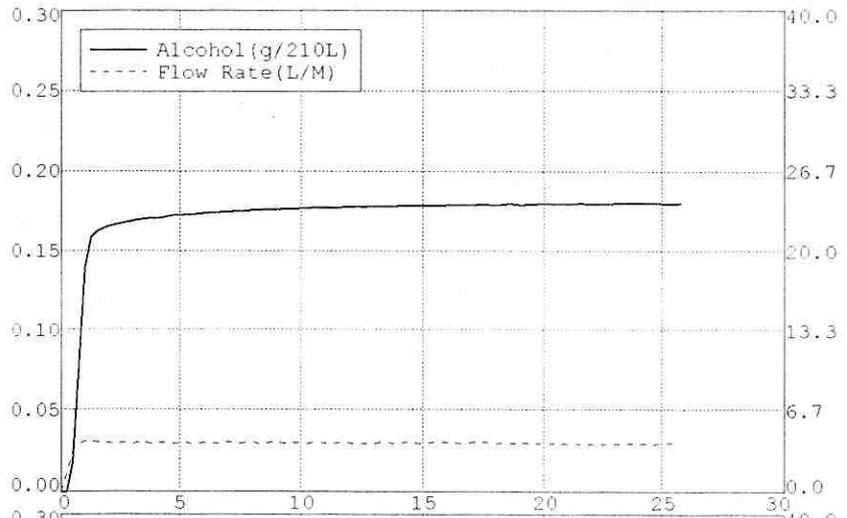

SERVICE AUTHORIZATION FORM
Highway Safety Technology Unit
 80 South Swan Street
 Albany, NY 12210
 Ph: 518-485-7636 / 518-402-0689
 Fax: 518-457-6869

*Mys
5/2/23*

THIS FORM IS USED TO AUTHORIZE THE DIVISION OF CRIMINAL JUSTICE SERVICES TO PERFORM SERVICE ON THE INSTRUMENT IDENTIFIED. THIS AUTHORIZATION MUST ACCOMPANY EACH PIECE OF EQUIPMENT WHEN IT IS PRESENTED TO THE EQUIPMENT REPAIR CENTER FOR SERVICE. **PLEASE SIGN AND DATE FORM.**

SECTION I - AGENCY INFORMATION

Name of Agency Lake George Park Commission		Today's Date <i>5-2-23</i>
Address 75 Fort George Rd.		City, State, ZIP Lake George, NY 12845
Contact Person		Contact Telephone 518-668-9347
Contact Email		Best Way to Reach You During Appointment Period

SECTION II - INSTRUMENT INFORMATION

Instrument Manufacturer (Please Circle) NPAS DMT GUTH Applied Concepts(Stalker) Decatur(Genesis) Kustom(Eagle/Falcon) MPH Alco-Sensor Other:		
Model Number Datamaster DMT		Instrument Serial Number 300391
Antenna Serial Number (if applicable) Antenna 1 -- / Antenna 2 --		Type of maintenance (check appropriate) <input checked="" type="checkbox"/> Calibration Check <input type="checkbox"/> Repair
Brief Description of Malfunction		
List all parts, cables and/or accessories being submitted. Tuning forks must accompany all radar units (if applicable). (Please Circle)		
DMT/SIM: DMT / SIM Tubes <i>1 Breath Hase</i> Keyboard / Other: <i>1 Sim Tubes</i>		Radar: Control Unit Antenna(s) Antenna Cable(s) Power Cord Forks Other: _
I acknowledge I am signing this Service Authorization Form as an act and deed of said agency, organization, or municipality, and that I am duly authorized to sign same for the uses and purposes mentioned herein. PLEASE SIGN AND DATE.		
Signature NA Re-Issue for Season		Date <i>KA. 5-2-23</i>

DCJS USE ONLY

Inspected instrument. Checked petco vs voltages front and remote operation. Performed calibration / adjustment procedure. Per subject, technician and diagnostic tests. Verified calibration. Opening cert for return.