



**CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS
MAINTAINED IN THE REGULAR COURSE OF BUSINESS**

I, **Steven J. Carluccio**, Highway Safety Equipment Technical Supervisor, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NATL PATENT ANALYTICAL SYSTEM, DATAMASTER DMT breath test instrument, serial number 300391, performed on October 24, 2023 by Office of Public Safety employee Jonathan Mascolo, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/ maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance /calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink that reads "Steven J. Carluccio".

Digitally signed under ESRA
by Steven J. Carluccio
on 11/08/2023 09:31 AM

Steven J. Carluccio
Highway Safety Equipment Technical Supervisor
Office of Public Safety

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Lake George Park Commission

Manufacturer: NATL PATENT ANALYTICAL SYSTEM

Model: DATAMASTER DMT

Serial Number: 300391

Date: October 24, 2023

Reference Solution Lot Number : 23050

Reference Solution Standard : 0.10% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.100 %	34.02 degrees centigrade
2	0.099 %	34.02 degrees centigrade
3	0.099 %	34.02 degrees centigrade
4	0.100 %	34.02 degrees centigrade

Reference Solution Lot Number : 23100

Reference Solution Standard : 0.08% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.080 %	34.02 degrees centigrade
2	0.078 %	34.02 degrees centigrade
3	0.078 %	34.02 degrees centigrade
4	0.079 %	34.02 degrees centigrade

Reference Solution Lot Number : 22450

Reference Solution Standard : 0.18% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.177 %	34.01 degrees centigrade
2	0.177 %	34.01 degrees centigrade
3	0.177 %	34.01 degrees centigrade
4	0.177 %	34.01 degrees centigrade

I hereby certify that I have performed any necessary maintenance procedures and calibrated NATL PATENT ANALYTICAL SYSTEM breath test instrument model DATAMASTER DMT, serial number 300391, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.


I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.

Performed by:



Digitally signed under ESRA
by Jonathan Mascolo
on 10/24/2023 02:51 PM

Reviewed by:

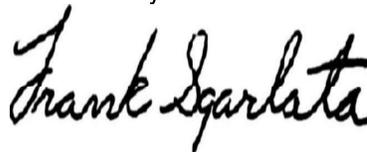

Digitally signed under ESRA
by Frank Sgarlata
on 10/24/2023 03:53 PM

Jonathan Mascolo
Highway Safety Equipment Technician
Breath Analysis Operator Permit #45339

Frank Sgarlata
Breath Analysis Technical Supervisor

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Lake George Park Commission
Manufacturer: NATL PATENT ANALYTICAL SYSTEM
Model: DATAMASTER DMT
Serial Number: 300391
Date: October 24, 2023

- 1. General appearance and condition of this device -----: **OK**

- 2. Check controls and indicators -----: **OK**

- 3. Check breath flow system -----: **OK**

- 4. Check printer operation -----: **OK**

- 5. System cycles through all modes -----: **OK**



6. Record any repairs made to this instrument and list services provided : INSPECTED INSTRUMENT, CHECKED SETUP VOLTAGES, PRINT AND REMOTE OPERATION. PERFORMED CALIBRATION/ADJUSTMENT PROCEDURE, RAN SUBJECT, TECHNICIAN AND DIAGNOSTIC TESTS, VERIFIED CALIBRATION.

Performed by:

Handwritten signature of Jonathan Mascolo in black ink.

Digitally signed under ESRA
by Jonathan Mascolo
on 10/24/2023 02:51 PM

Reviewed by:

Handwritten signature of Frank Sgarlata in black ink.

Digitally signed under ESRA
by Frank Sgarlata
on 10/24/2023 03:53 PM

Jonathan Mascolo
Highway Safety Equipment Technician
Breath Analysis Operator Permit #45339

Frank Sgarlata
Breath Analysis Technical Supervisor

TECHNICIAN TEST

LAKE GEORGE
PARK COMMISSION
DATAMASTER dmt: 300391




Date: 10/24/2023

OPERATOR NAME:
JONATHAN M MASCOLO
Permit #: 45339
Operator Agency/Dept: LAKE GEORGE PK COMM
Reference Standard #: 23100

Nominal = 0.080 g/210L

BLANK TEST	0.000	09:51
INTERNAL STANDARD	VERIFIED	09:51
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.080	09:52
BLANK TEST	0.000	09:53
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.078	09:53
BLANK TEST	0.000	09:54
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.078	09:54
BLANK TEST	0.000	09:55
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.079	09:55
BLANK TEST	0.000	09:56

Average = 0.0788
Std Dev = 0.0010

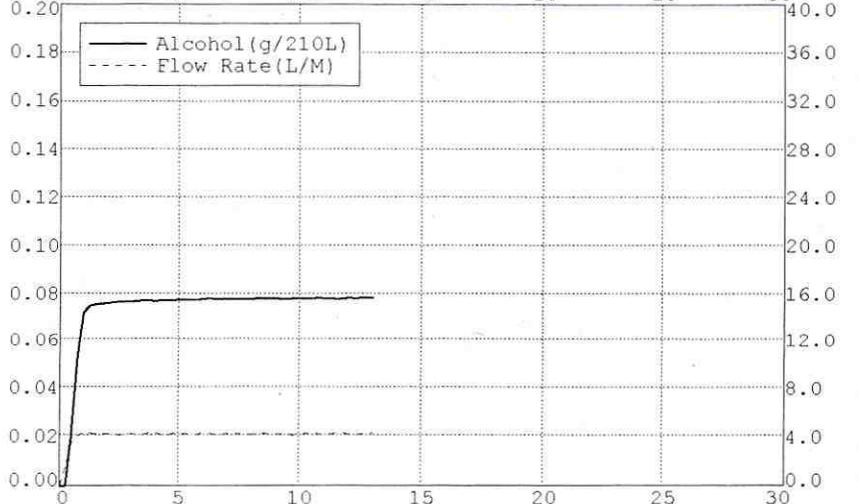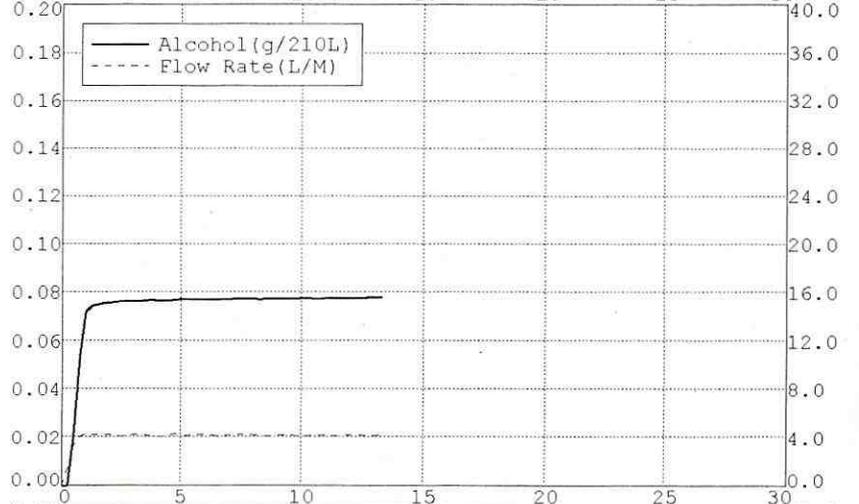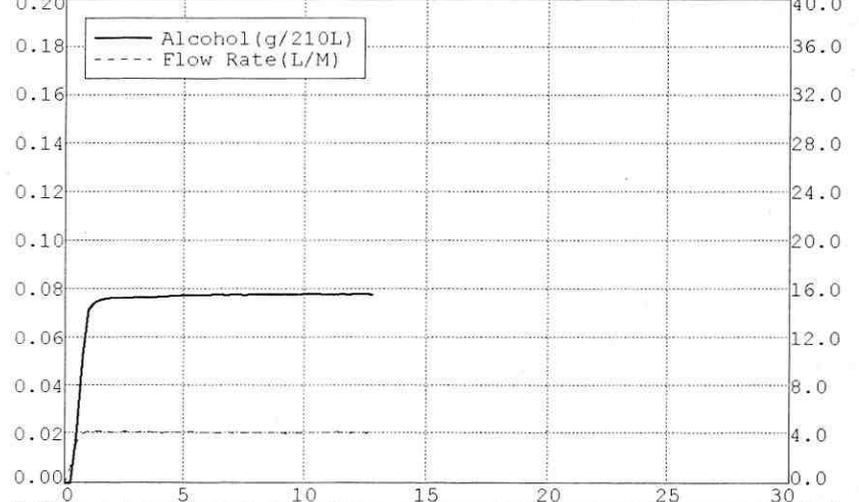

TECHNICIAN TEST

LAKE GEORGE
 PARK COMMISSION
 DATAMASTER dmt: 300391





Date: 10/24/2023

OPERATOR NAME:
 JONATHAN M MASCOLO
 Permit #: 45339
 Operator Agency/Dept: LAKE GEORGE PK COMM
 Reference Standard #: 23050

Nominal = 0.100 g/210L

BLANK TEST	0.000	09:58
INTERNAL STANDARD	VERIFIED	09:58
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.100	09:59
BLANK TEST	0.000	09:59
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.099	10:00
BLANK TEST	0.000	10:01
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.099	10:01
BLANK TEST	0.000	10:02
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.100	10:02
BLANK TEST	0.000	10:03

Average = 0.0995
 Std Dev = 0.0006

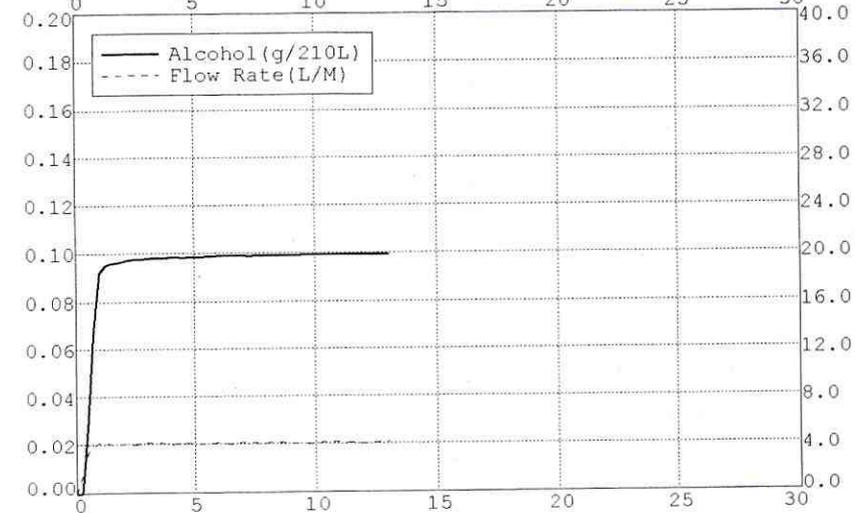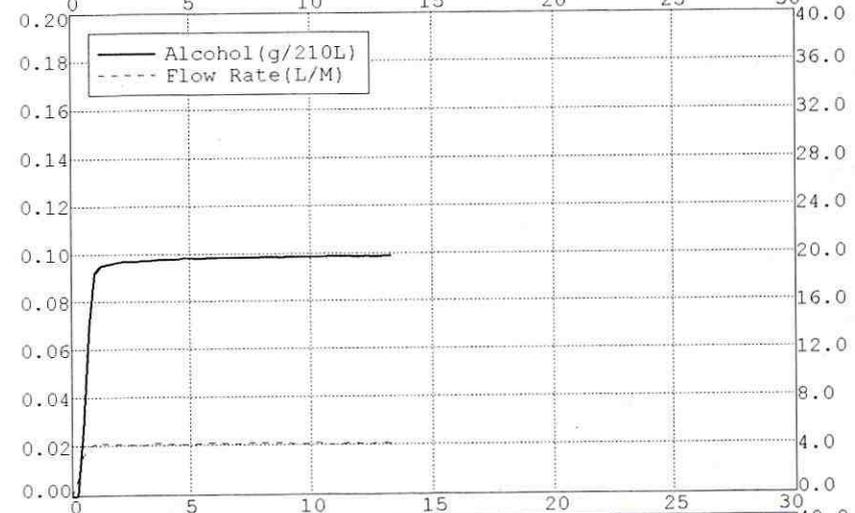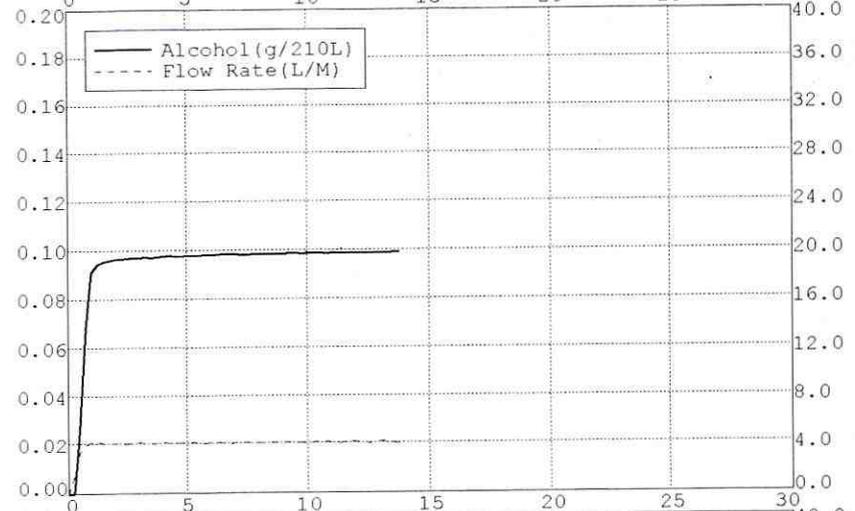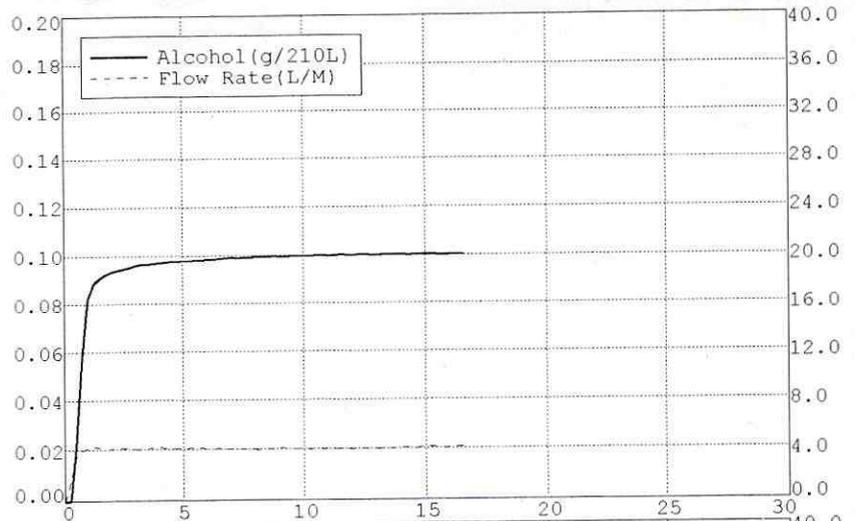

TECHNICIAN TEST

LAKE GEORGE
 PARK COMMISSION
 DATAMASTER dmt: 300391





Date: 10/24/2023

OPERATOR NAME:
 JONATHAN M MASCOLO
 Permit #: 45339
 Operator Agency/Dept: LAKE GEORGE PK COMM
 Reference Standard #: 22450

Nominal = 0.180 g/210L

BLANK TEST	0.000	10:07
INTERNAL STANDARD	VERIFIED	10:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.177	10:08
BLANK TEST	0.000	10:08
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.177	10:09
BLANK TEST	0.000	10:10
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.177	10:10
BLANK TEST	0.000	10:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.177	10:11
BLANK TEST	0.000	10:12

Average = 0.1770
 Std Dev = 0.0000

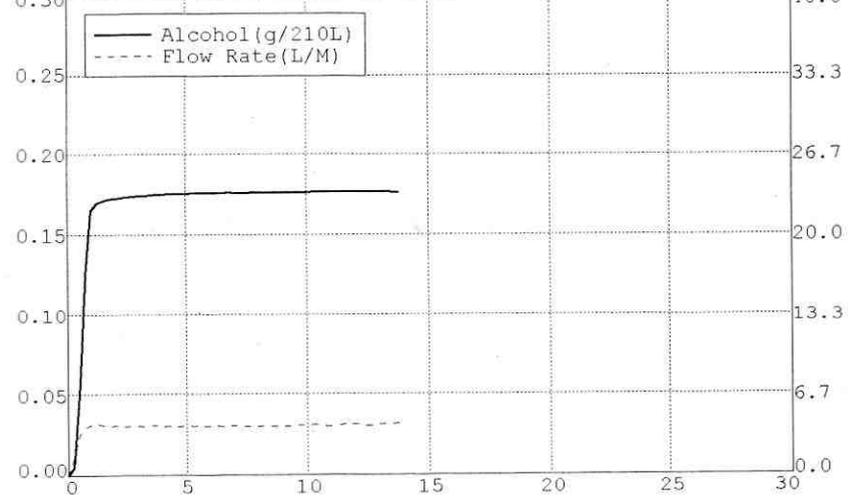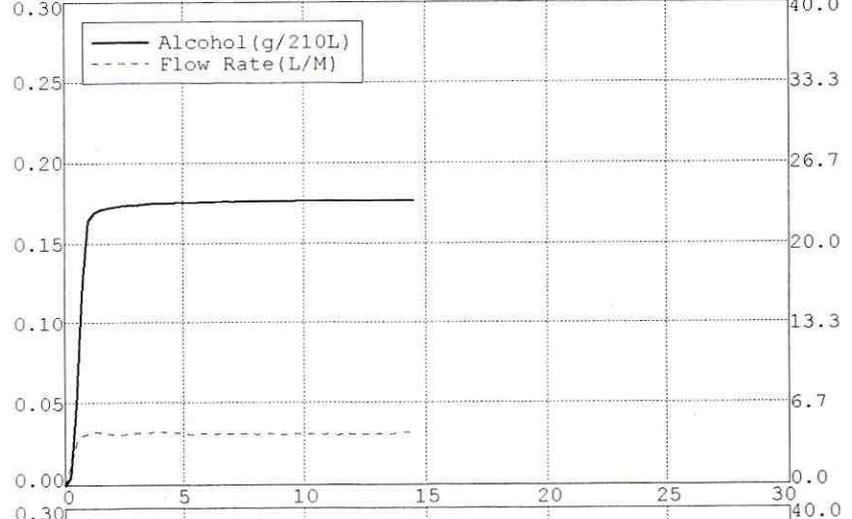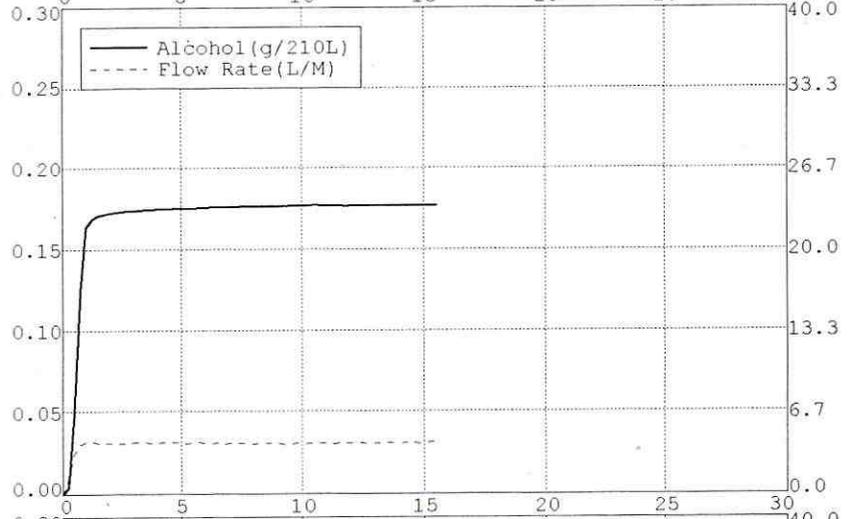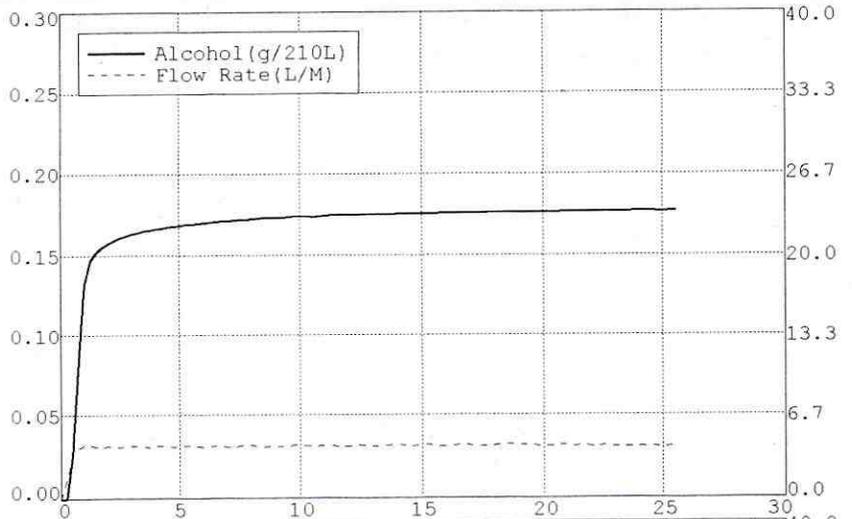

*10-24-2023

SERVICE AUTHORIZATION FORM
Highway Safety Technology Unit
 80 South Swan Street
 Albany, NY 12210
 Ph: 518-485-7636 / 518-402-0689
 Fax: 518-457-6869

THIS FORM IS USED TO AUTHORIZE THE DIVISION OF CRIMINAL JUSTICE SERVICES TO PERFORM SERVICE ON THE INSTRUMENT IDENTIFIED. THIS AUTHORIZATION MUST ACCOMPANY EACH PIECE OF EQUIPMENT WHEN IT IS PRESENTED TO THE EQUIPMENT REPAIR CENTER FOR SERVICE. **PLEASE SIGN AND DATE FORM.**

SECTION I - AGENCY INFORMATION

Name of Agency <i>Lake George Park Commission</i>		Today's Date
Address <i>75 Fort George Rd</i>		City, State, ZIP <i>Lake George NY 12845</i>
Contact Person <i>Lt. Joe Johns</i>		Contact Telephone <i>518-668-9347</i>
Contact Email <i>jjohns@lgpc.state.ny.us</i>		Best Way to Reach You During Appointment Period

SECTION II - INSTRUMENT INFORMATION

Instrument Manufacturer (Please Circle) NPAS DMT GUTH Applied Concepts(Stalker) Decatur(Genesis) Kustom(Eagle/Falcon) MPH Alco-Sensor Other:		
Model Number <i>Data Master DMT</i>		Instrument Serial Number <i>300391</i>
Antenna Serial Number (if applicable) Antenna 1 - / Antenna 2 -		Type of maintenance (check appropriate) <input type="checkbox"/> Calibration Check <input type="checkbox"/> Repair
Brief Description of Malfunction		
List all parts, cables and/or accessories being submitted. Tuning forks must accompany all radar units (if applicable). (Please Circle)		
DMT/SIM: DMT <i>0*</i> SIM Tubes <i>0* Simulator tube</i> Other:		Radar: Control Unit Antenna(s) Antenna Cable(s) Power Cord Forks Other:
I acknowledge I am signing this Service Authorization Form as an act and deed of said agency, organization, or municipality, and that I am duly authorized to sign same for the uses and purposes mentioned herein. PLEASE SIGN AND DATE.		
Signature <i>Lt. Joe Johns</i>		Date <i>10/20/23</i>

DCJS USE ONLY

*Inspected instrument, checked setup voltages, print and remote operation. Performed calibration/adjustment procedure, ran subject, technician and diagnostic tests, verified calibration. * @ 10-24-2023*