



---

**CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS  
MAINTAINED IN THE REGULAR COURSE OF BUSINESS**

I, **Martin Schilling, Highway Safety Equipment Technician 2, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210**, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NATL PATENT ANALYTICAL SYSTEM, DATAMASTER DMT breath test instrument, serial number 300391, performed on March 25, 2024 by Office of Public Safety employee Jonathan Mascolo, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/ maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance /calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink that reads "Martin Schilling".

Digitally signed under ESRA  
by Martin Schilling  
on 03/26/2024 11:44 AM

---

**Martin Schilling  
Highway Safety Equipment Technician 2  
Office of Public Safety**

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

**Name of Submitting Agency: Lake George Park Commission**

**Manufacturer: NATL PATENT ANALYTICAL SYSTEM**

**Model: DATAMASTER DMT**

**Serial Number: 300391**

**Date: March 25, 2024**

**Reference Solution Lot Number : 23451**

**Reference Solution Standard : 0.10% at 34.0 degrees centigrade**

Test No	Test Result	Simulator Temperature
1	0.101 %	34.00 degrees centigrade
2	0.100 %	34.00 degrees centigrade
3	0.100 %	34.00 degrees centigrade
4	0.101 %	34.00 degrees centigrade

**Reference Solution Lot Number : 23100**

**Reference Solution Standard : 0.08% at 34.0 degrees centigrade**

Test No	Test Result	Simulator Temperature
1	0.081 %	34.02 degrees centigrade
2	0.080 %	34.02 degrees centigrade
3	0.081 %	34.02 degrees centigrade
4	0.081 %	34.02 degrees centigrade

**Reference Solution Lot Number : 23380**

**Reference Solution Standard : 0.18% at 34.0 degrees centigrade**

Test No	Test Result	Simulator Temperature
1	0.178 %	34.01 degrees centigrade
2	0.178 %	34.01 degrees centigrade
3	0.178 %	34.01 degrees centigrade
4	0.178 %	34.01 degrees centigrade

I hereby certify that I have performed any necessary maintenance procedures and calibrated NATL PATENT ANALYTICAL SYSTEM breath test instrument model DATAMASTER DMT, serial number 300391, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.


I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.

Performed by:



Digitally signed under ESRA  
by Jonathan Mascolo  
on 03/25/2024 01:56 PM

Reviewed by:

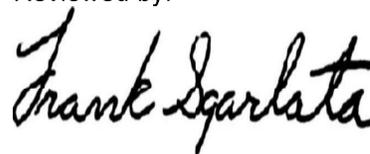

Digitally signed under ESRA  
by Frank Sgarlata  
on 03/26/2024 06:25 AM

**Jonathan Mascolo**  
**Highway Safety Equipment Technician**  
**Breath Analysis Operator Permit #45339**

**Frank Sgarlata**  
**Breath Analysis Technical Supervisor**

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

**Name of Submitting Agency: Lake George Park Commission**  
**Manufacturer: NATL PATENT ANALYTICAL SYSTEM**  
**Model: DATAMASTER DMT**  
**Serial Number: 300391**  
**Date: March 25, 2024**

- 1. General appearance and condition of this device -----: **OK**
  
- 2. Check controls and indicators -----: **OK**
  
- 3. Check breath flow system -----: **OK**
  
- 4. Check printer operation -----: **OK**
  
- 5. System cycles through all modes -----: **OK**



**6. Record any repairs made to this instrument and list services provided : INSPECTED INSTRUMENT, CHECKED SETUP VOLTAGES, PRINT AND REMOTE OPERATION. PERFORMED CALIBRATION/ADJUSTMENT PROCEDURE, RAN SUBJECT, TECHNICIAN AND DIAGNOSTIC TESTS, VERIFIED CALIBRATION.**

**THIS CERTIFICATE EXPIRES 365 DAYS FROM THE DATE AT THE TOP OF THIS PAGE.**

Performed by:

Handwritten signature of Jonathan Mascolo in black ink.

Digitally signed under ESRA  
by Jonathan Mascolo  
on 03/25/2024 01:56 PM

Reviewed by:

Handwritten signature of Frank Sgarlata in black ink.

Digitally signed under ESRA  
by Frank Sgarlata  
on 03/26/2024 06:25 AM

---

**Jonathan Mascolo**  
**Highway Safety Equipment Technician**  
**Breath Analysis Operator Permit #45339**

---

**Frank Sgarlata**  
**Breath Analysis Technical Supervisor**

TECHNICIAN TEST

LAKE GEORGE  
 PARK COMMISSION  
 DATAMASTER dmt: 300391





Date: 03/25/2024

OPERATOR NAME:  
 JONATHAN M MASCOLO  
 Permit #: 45339  
 Operator Agency/Dept: LAKE GEORGE PK COMM  
 Reference Standard #: 23100

Nominal = 0.080 g/210L

BLANK TEST	0.000	13:03
INTERNAL STANDARD	VERIFIED	13:03
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.081	13:03
BLANK TEST	0.000	13:04
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.080	13:04
BLANK TEST	0.000	13:05
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.081	13:05
BLANK TEST	0.000	13:06
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.081	13:07
BLANK TEST	0.000	13:08

Average = 0.0808  
 Std Dev = 0.0005

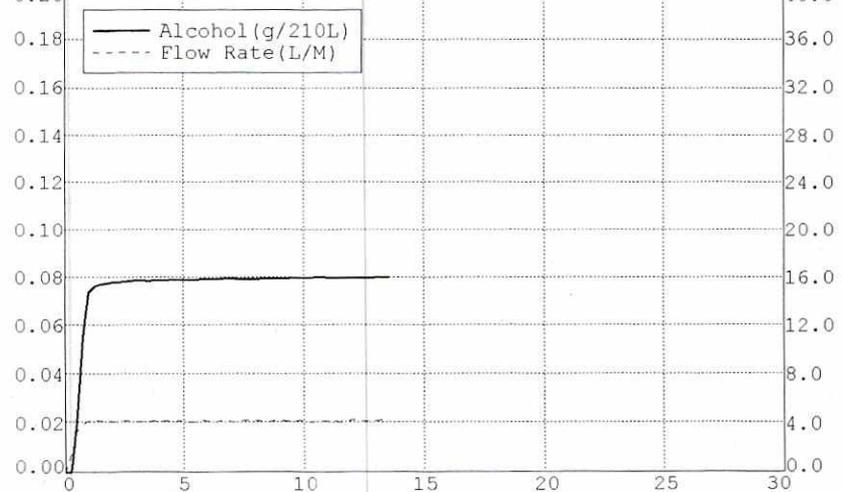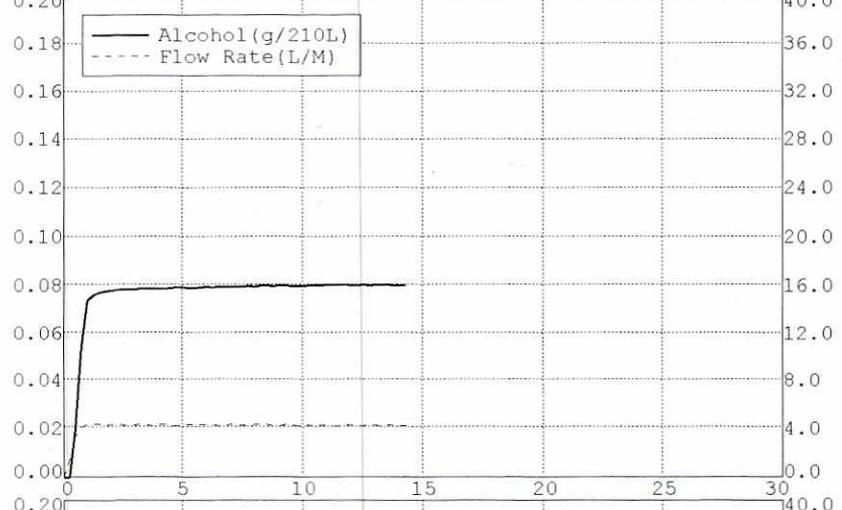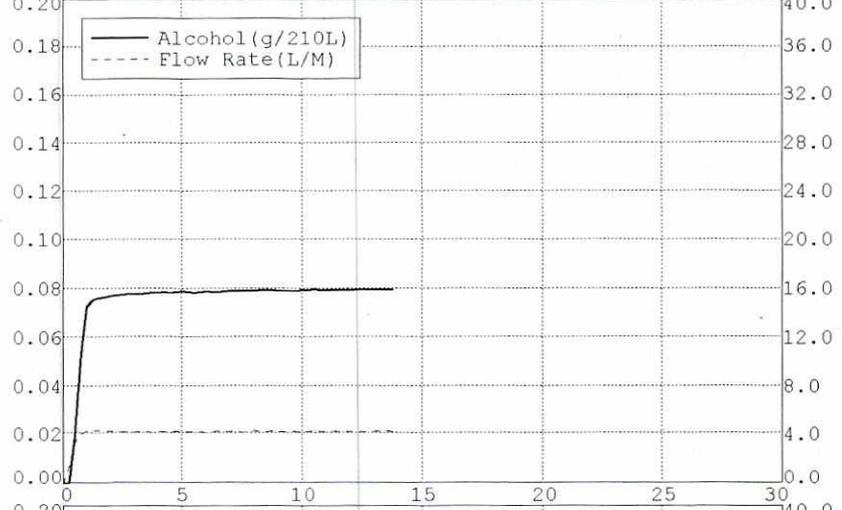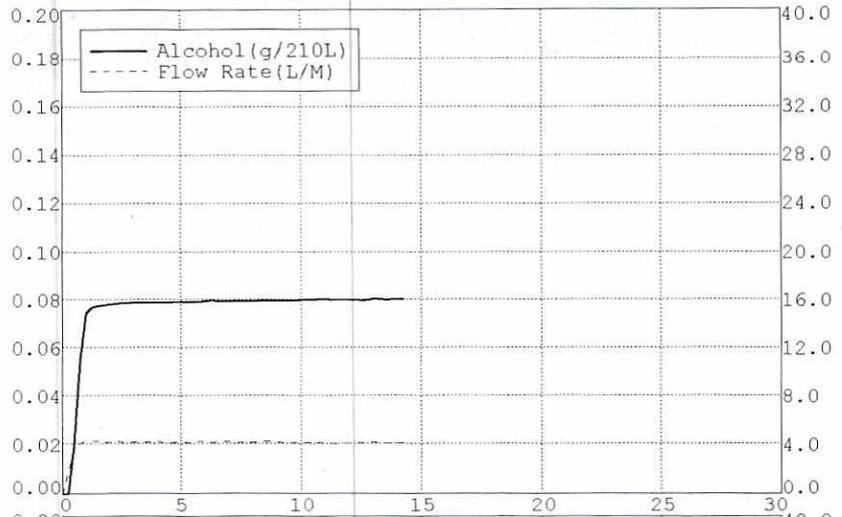

TECHNICIAN TEST

LAKE GEORGE  
PARK COMMISSION  
DATAMASTER dmt: 300391





Date: 03/25/2024

OPERATOR NAME:  
JONATHAN M MASCOLO  
Permit #: 45339  
Operator Agency/Dept: LAKE GEORGE PK COMM  
Reference Standard #: 23451

Nominal = 0.100 g/210L

BLANK TEST	0.000	12:55
INTERNAL STANDARD	VERIFIED	12:55
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.101	12:56
BLANK TEST	0.000	12:57
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.100	12:57
BLANK TEST	0.000	12:58
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.100	12:58
BLANK TEST	0.000	12:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.101	13:00
BLANK TEST	0.000	13:00

Average = 0.1005  
Std Dev = 0.0006

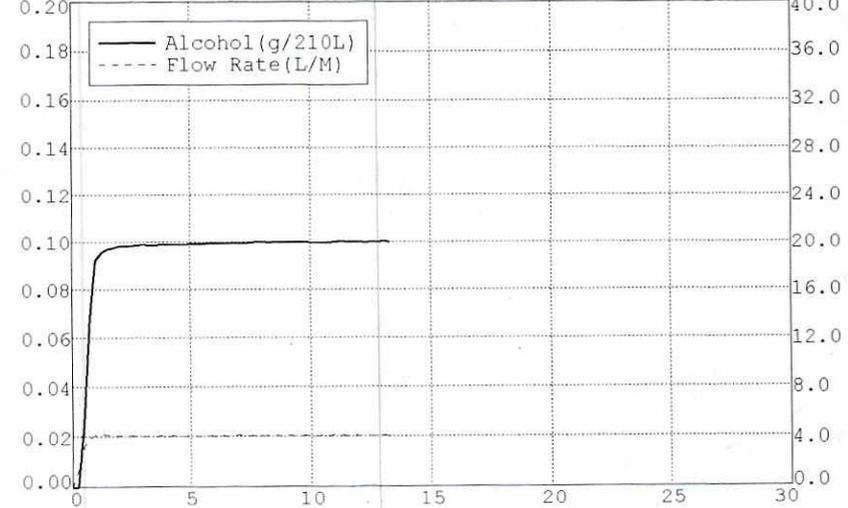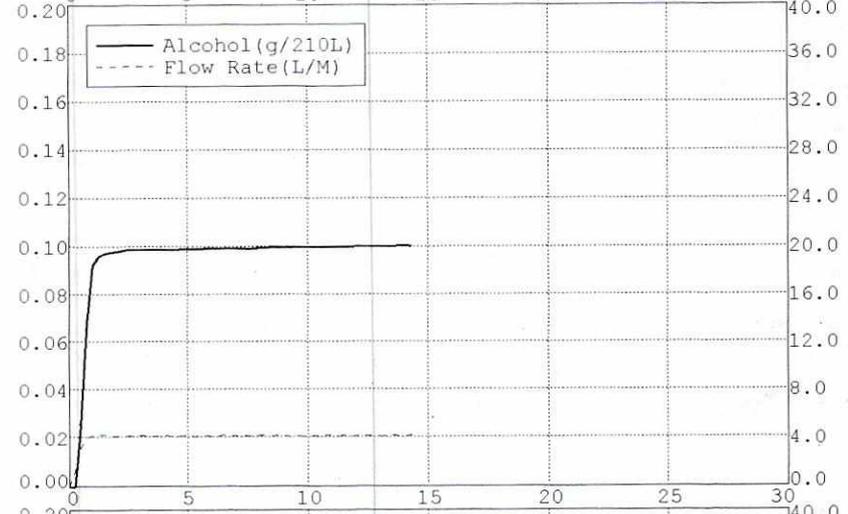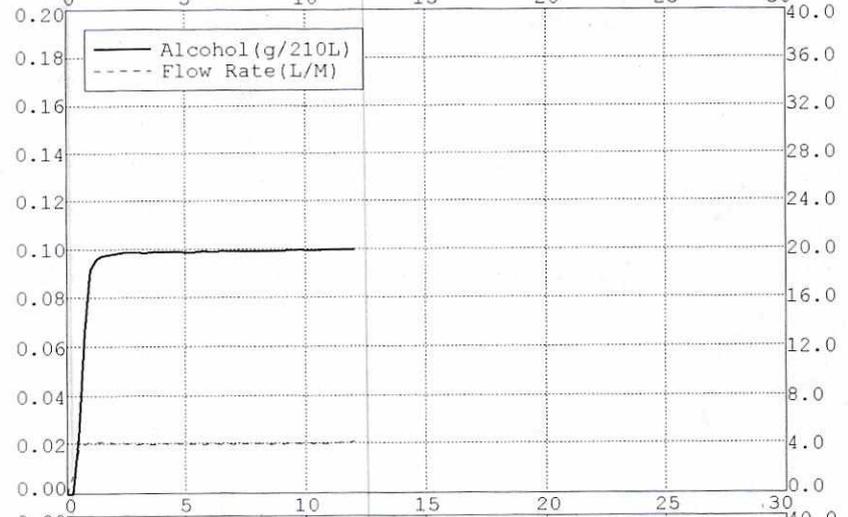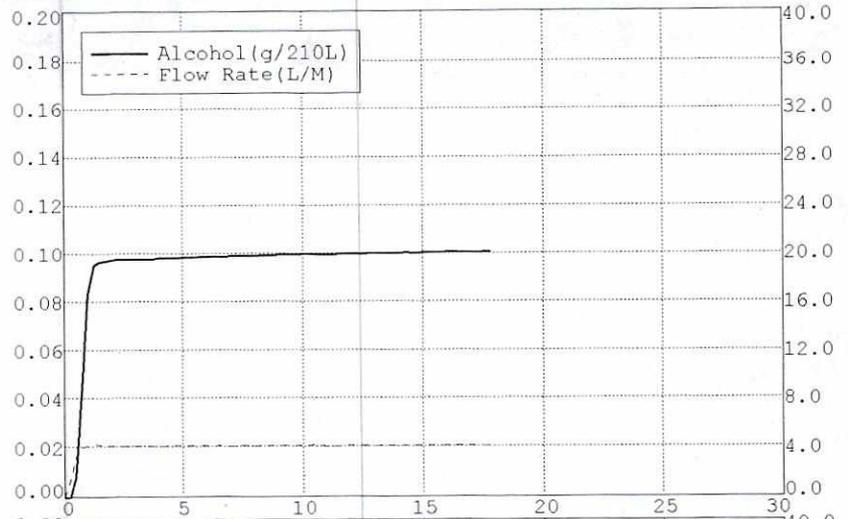

TECHNICIAN TEST

LAKE GEORGE  
 PARK COMMISSION  
 DATAMASTER dmt: 300391





Date: 03/25/2024

OPERATOR NAME:  
 JONATHAN M MASCOLO  
 Permit #: 45339  
 Operator Agency/Dept: LAKE GEORGE PK COMM  
 Reference Standard #: 23380

Nominal = 0.180 g/210L

BLANK TEST	0.000	13:10
INTERNAL STANDARD	VERIFIED	13:10
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.178	13:10
BLANK TEST	0.000	13:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.178	13:12
BLANK TEST	0.000	13:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.178	13:13
BLANK TEST	0.000	13:14
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.178	13:14
BLANK TEST	0.000	13:15

Average = 0.1780  
 Std Dev = 0.0000

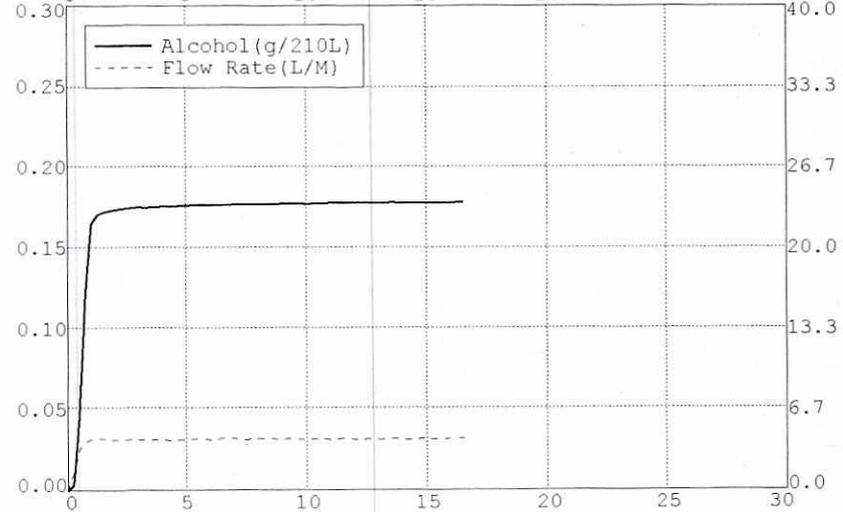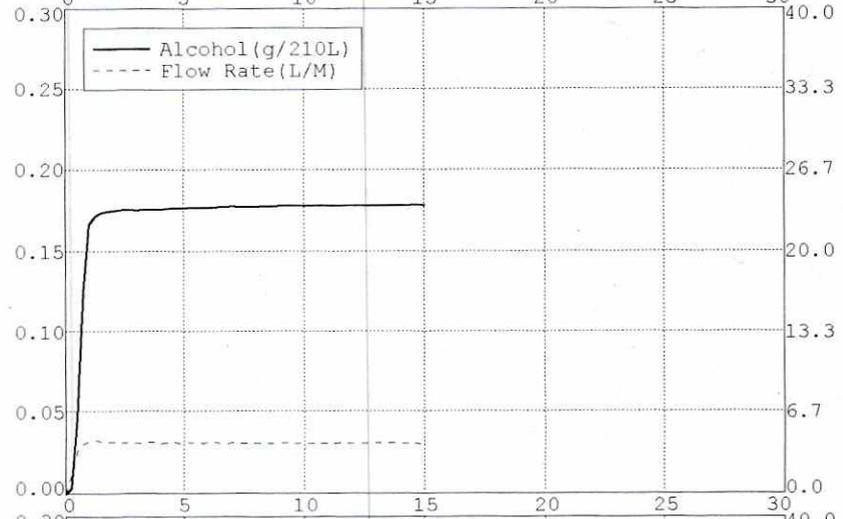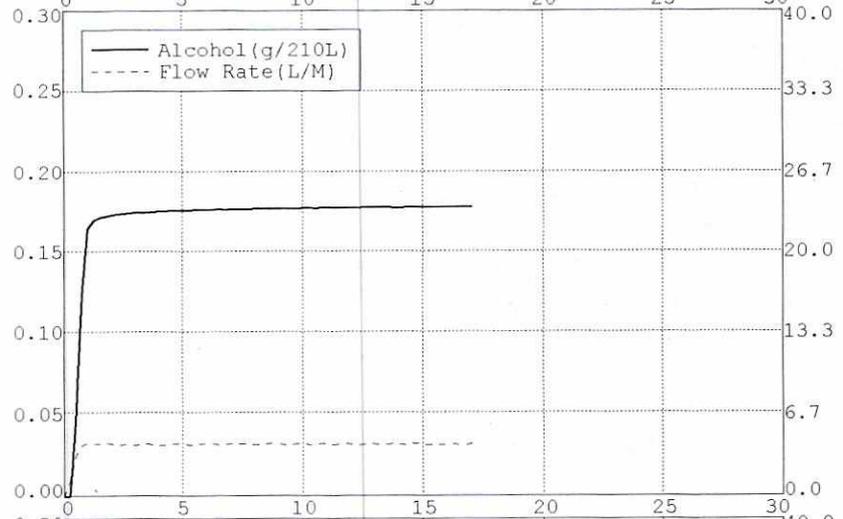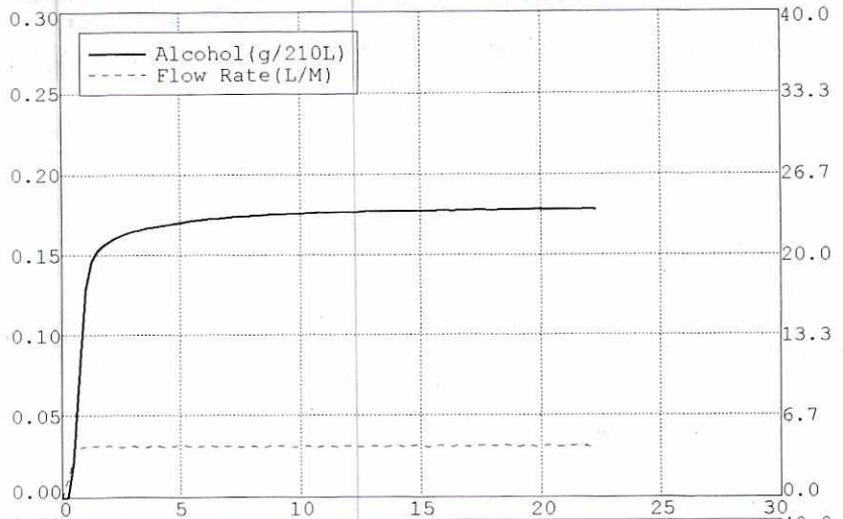

**SERVICE AUTHORIZATION FORM**  
**Highway Safety Technology Unit**  
**80 South Swan Street**  
**Albany, NY 12210**  
**Ph: 518-485-7636 / 518-402-0689**  
**Fax: 518-457-6869**

THIS FORM IS USED TO AUTHORIZE THE DIVISION OF CRIMINAL JUSTICE SERVICES TO PERFORM SERVICE ON THE INSTRUMENT IDENTIFIED. THIS AUTHORIZATION MUST ACCOMPANY EACH PIECE OF EQUIPMENT WHEN IT IS PRESENTED TO THE EQUIPMENT REPAIR CENTER FOR SERVICE. **PLEASE SIGN AND DATE FORM.**

**SECTION I - AGENCY INFORMATION**

Name of Agency <b>Lake George Park Commission</b>		Today's Date <b>3/25/2024</b>
Address	City, State, ZIP	
Contact Person	Contact Telephone	
Contact Email	Best Way to Reach You During Appointment Period	

**SECTION II - INSTRUMENT INFORMATION**

Instrument Manufacturer (Please Circle) <input checked="" type="checkbox"/> NPAS DMT <input type="checkbox"/> GUTH <input type="checkbox"/> Applied Concepts (Stalker) <input type="checkbox"/> Decatur (Genesis) <input type="checkbox"/> Kustom (Eagle/Falcon) <input type="checkbox"/> MPH <input type="checkbox"/> Alco-Sensor <input type="checkbox"/> Other:		
Model Number <b>Datamaster DMT</b>	Instrument Serial Number <b>300391</b>	
Antenna Serial Number (if applicable) Antenna 1 - <b>n/a</b> /      Antenna 2 - <b>n/a</b>	Type of maintenance (check appropriate) <input checked="" type="checkbox"/> Calibration Check <input type="checkbox"/> Repair	
Brief Description of Malfunction		
List all parts, cables and/or accessories being submitted. Tuning forks must accompany all radar units (if applicable). (Please Circle)		
DMT/SIM: DMT <input checked="" type="checkbox"/> SIM    Tubes <input checked="" type="checkbox"/> <b>breath tube</b> Keyboard <input checked="" type="checkbox"/> Other: <input checked="" type="checkbox"/> <b>Power cable</b> <input checked="" type="checkbox"/> <b>simulator tube</b>	Radar:	Antenna(s)
	Control Unit	Antenna Cable(s)
	Power Cord	Forks
		Other: _
I acknowledge I am signing this Service Authorization Form as an act and deed of said agency, organization, or municipality, and that I am duly authorized to sign same for the uses and purposes mentioned herein. <b>PLEASE SIGN AND DATE.</b>		
Signature <b>n/a</b>	Date <b>n/a</b>	

**DCJS USE ONLY**

*Inspected instrument, checked setup voltages, print and remote operation. Performed calibration/adjustment procedure, ran subject, technician and diagnostic tests, verified calibration \*e 3-25-24*