



Division of Criminal Justice Services

CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS MAINTAINED IN THE REGULAR COURSE OF BUSINESS

I, Joshua Vinehout, Supervisor of Public Safety Programs, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NAT'L PATENT ANALYTICAL SYS, DATAMASTER DMT breath test instrument, serial number 105208, performed on March 31, 2021 by Office of Public Safety employee Martin Schilling, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/ maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance /calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink that reads "Joshua Vinehout".

Digitally signed under
ESRA by Joshua Vinehout
on 4/7/2021 12:26 PM

Joshua Vinehout
Supervisor of Public Safety Programs
Office of Public Safety

An Equal Opportunity/Affirmative Action Agency

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Warren County Sheriff's Office

Manufacturer: NAT'L PATENT ANALYTICAL SYS

Model: DATAMASTER DMT

Date: March 31, 2021

Serial Number: 105208

Reference Solution Lot Number: 20361

Reference Solution Standard: 0.10 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.097 %	34.01 degrees centigrade
2	0.097 %	34.00 degrees centigrade
3	0.097 %	34.01 degrees centigrade
4	0.097 %	34.01 degrees centigrade

Reference Solution Lot Number: 20470

Reference Solution Standard: 0.08 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.080 %	34.00 degrees centigrade
2	0.080 %	34.01 degrees centigrade
3	0.080 %	34.01 degrees centigrade
4	0.080 %	34.00 degrees centigrade

Reference Solution Lot Number: 20290

Reference Solution Standard: 0.180 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.183 %	34.00 degrees centigrade
2	0.183 %	34.00 degrees centigrade
3	0.183 %	34.01 degrees centigrade
4	0.183 %	34.01 degrees centigrade

I hereby certify that I have performed any necessary maintenance procedures and calibrated NAT'L PATENT ANALYTICAL SYS breath test instrument model DATAMASTER DMT, serial number 105208, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.

I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.

Performed by:



Digitally signed under
ESRA by Martin Schilling
on 3/31/2021 9:19 AM

Martin Schilling
Highway Safety Equipment Technician
Breath Analysis Operator Permit # 45926

Reviewed by:



Digitally signed under
ESRA by Frank Sgarlata
on 4/1/2021 1:28 PM

Frank Sgarlata
Breath Analysis Technical Supervisor

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Warren County Sheriff's Office
Manufacturer: NAT'L PATENT ANALYTICAL SYS
Model: DATAMASTER DMT
Serial Number: 105208
Date: March 31, 2021

**1. General Appearance and condition of this device -----: Reference Standard
0.00 and blank error**

2. Check controls and indicators -----: OK

3. Check breath flow system -----: OK

4. Check printer operation -----: OK



**Division of Criminal
Justice Services**

5. System cycles through all modes -----: OK

6. Record any repairs made to this instrument and list services provided: Cleaned 5Way and plunger. CHECKED SETUP VOLTAGES PRINT AND REMOTE OPERATION. PERFORMED CALIBRATION/ADJUSTMENT PROCEDURE, RAN SUBJECT, TECHNICIAN AND DIAGNOSTIC TESTS, VERIFIED CALIBRATION

Performed by:

A handwritten signature in black ink, appearing to read "Martin Schilling".

Digitally signed under
ESRA by Martin Schilling
on 3/31/2021 9:19 AM

Martin Schilling
Highway Safety Equipment Technician
Breath Analysis Operator Permit # 45926

Reviewed by:

A handwritten signature in black ink, appearing to read "Frank Sgarlata".

Digitally signed under
ESRA by Frank Sgarlata
on 4/1/2021 1:28 PM

Frank Sgarlata
Breath Analysis Technical Supervisor

TECHNICIAN TEST

WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 105208





Date: 03/31/2021

OPERATOR NAME:
 MARTIN J SCHILLING
 Permit #: 45926
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 20361

Nominal = 0.100 g/210L

BLANK TEST	0.000	07:56
INTERNAL STANDARD	VERIFIED	07:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.097	07:57
BLANK TEST	0.000	07:57
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.097	07:58
BLANK TEST	0.000	07:59
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.097	07:59
BLANK TEST	0.000	08:00
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.097	08:00
BLANK TEST	0.000	08:01

Average = 0.0970
 Std Dev = 0.0000

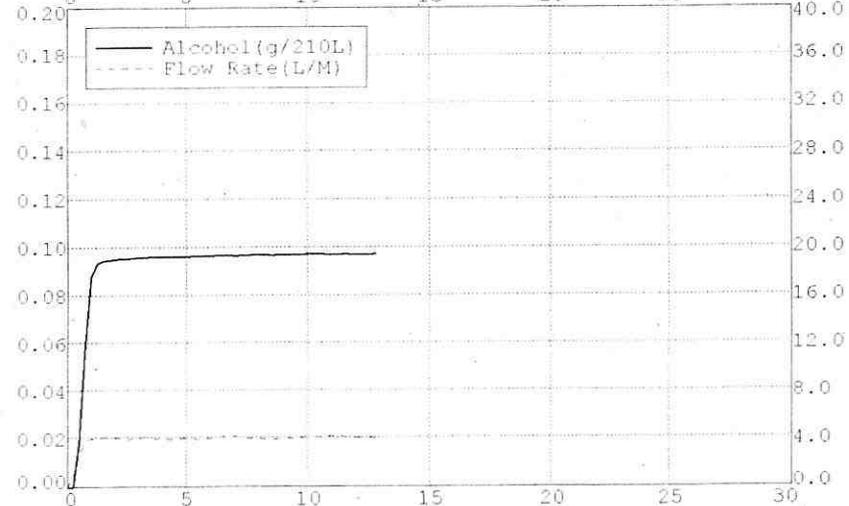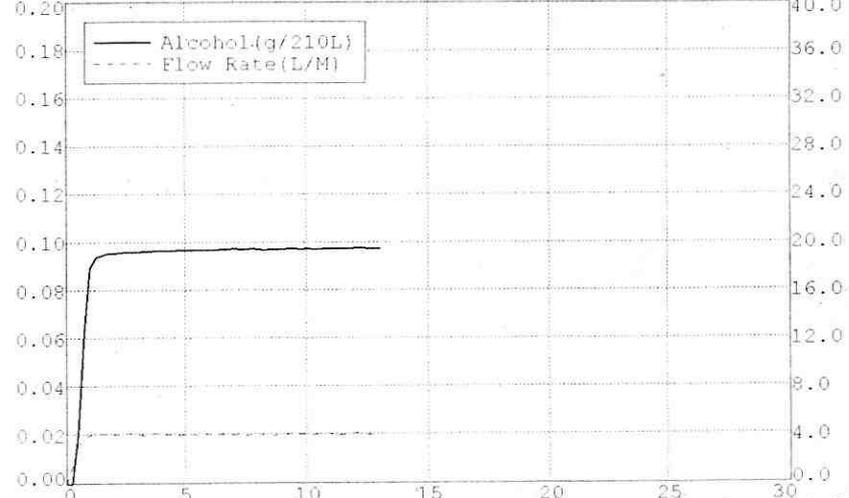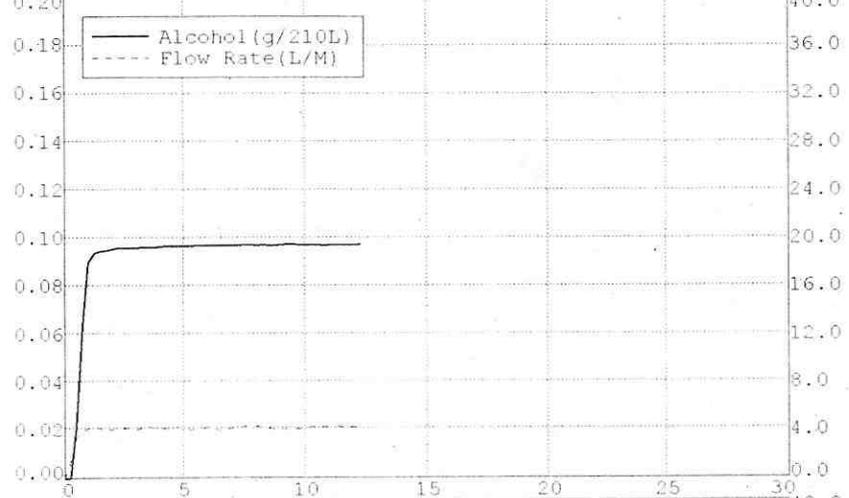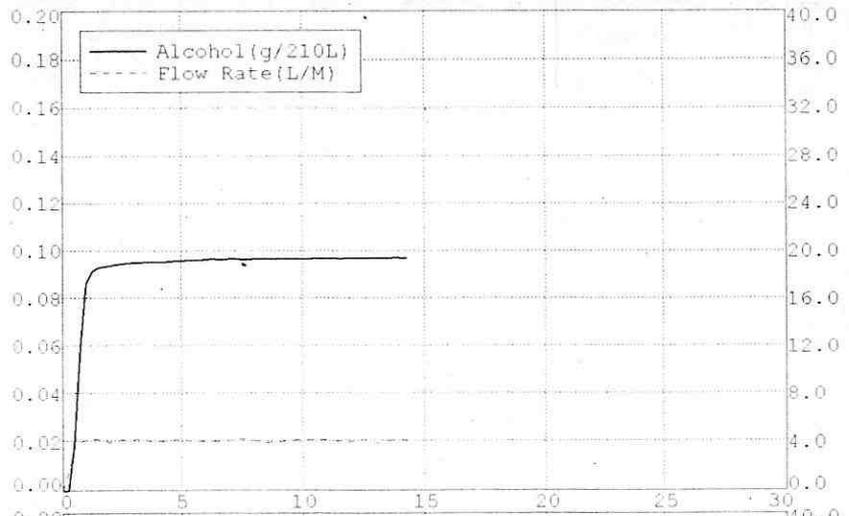

TECHNICIAN TEST

WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 105208





Date: 03/31/2021

OPERATOR NAME:
 MARTIN J SCHILLING
 Permit #: 45926
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 20470

Nominal = 0.080 g/210L

BLANK TEST	0.000	08:04
INTERNAL STANDARD	VERIFIED	08:05
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.080	08:05
BLANK TEST	0.000	08:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.080	08:06
BLANK TEST	0.000	08:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.080	08:07
BLANK TEST	0.000	08:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.080	08:08
BLANK TEST	0.000	08:09

Average = 0.0800
 Std Dev = 0.0000

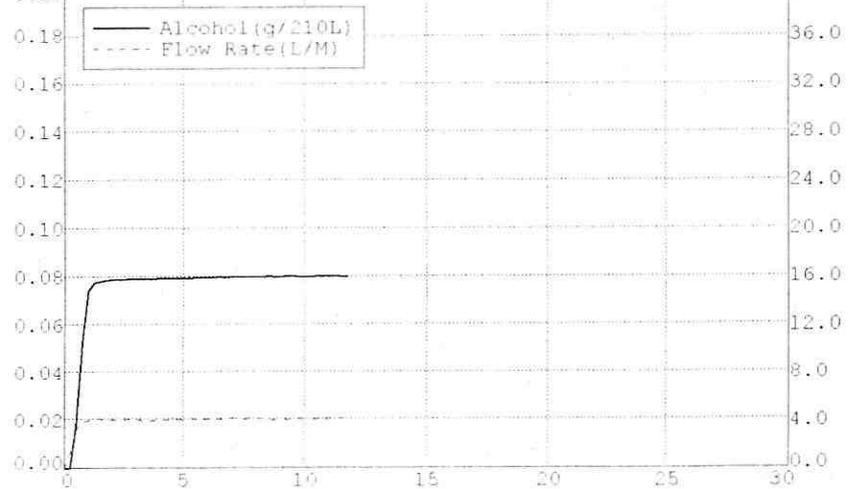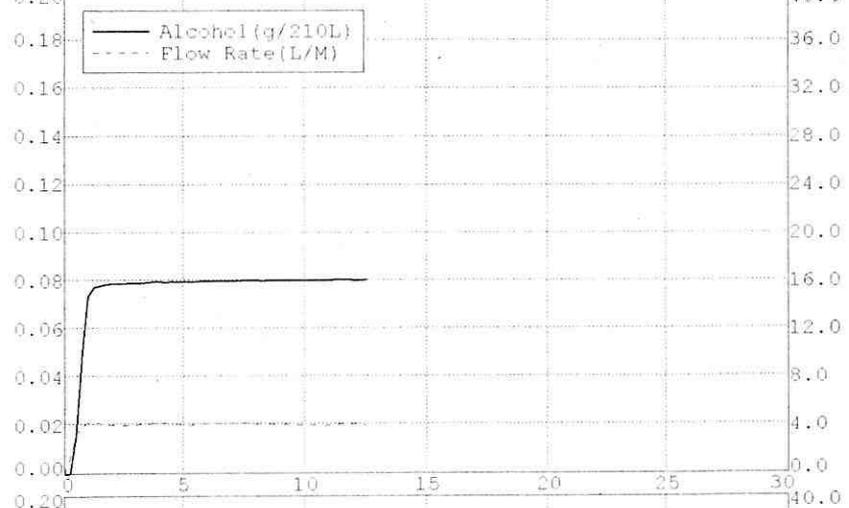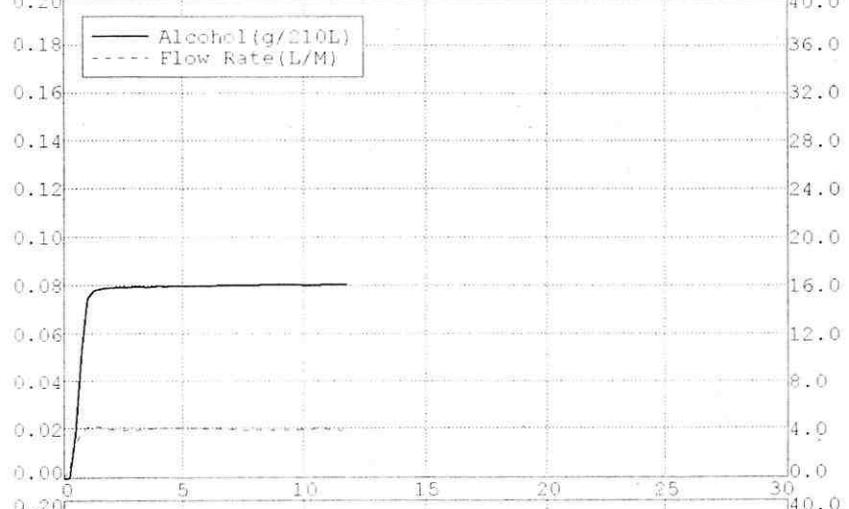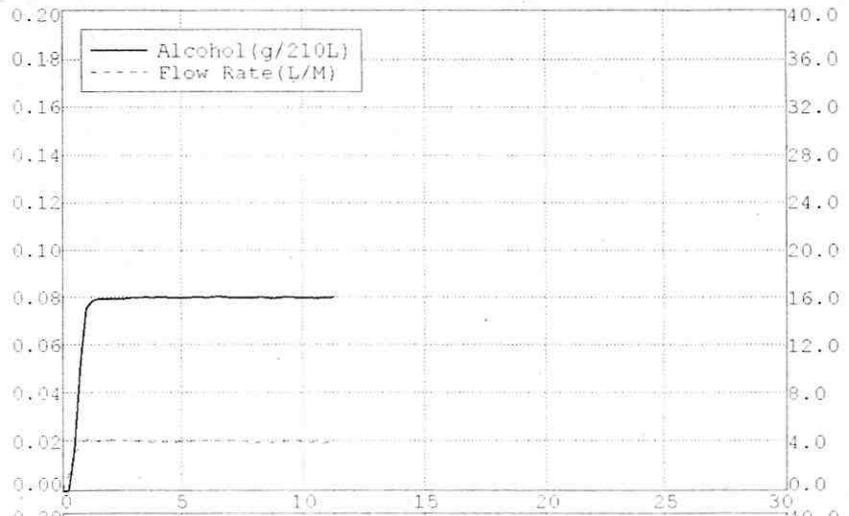

TECHNICIAN TEST

WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208





Date: 03/31/2021

OPERATOR NAME:
MARTIN J SCHILLING
Permit #: 45926
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20290

Nominal = 0.180 g/210L

BLANK TEST	0.000	08:12
INTERNAL STANDARD	VERIFIED	08:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.183	08:12
BLANK TEST	0.000	08:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.183	08:14
BLANK TEST	0.000	08:15
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.183	08:15
BLANK TEST	0.000	08:16
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.183	08:16
BLANK TEST	0.000	08:17

Average = 0.1830
Std Dev = 0.0000

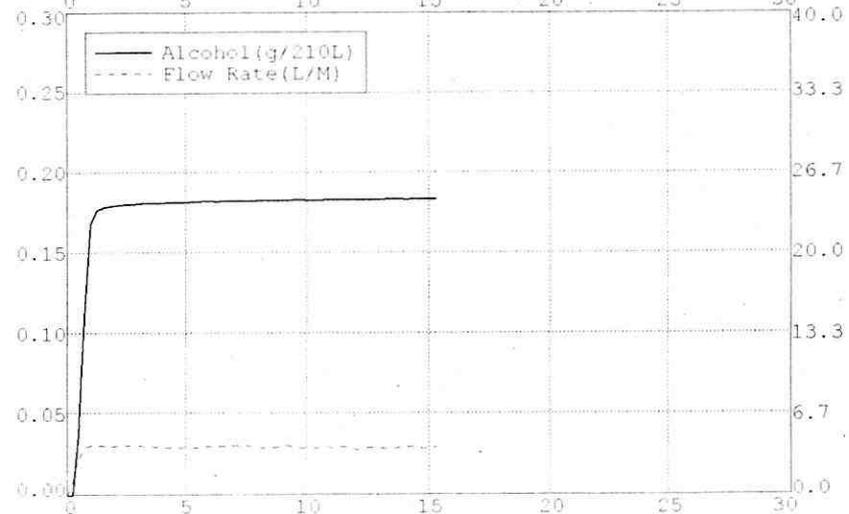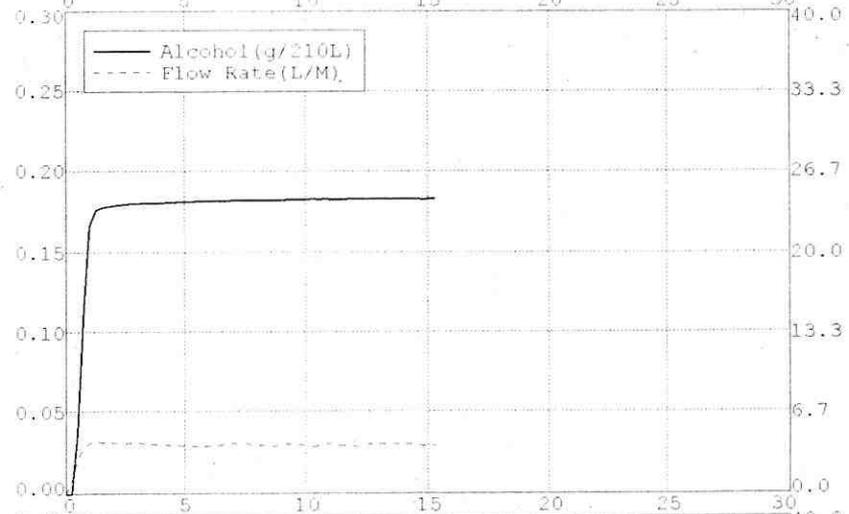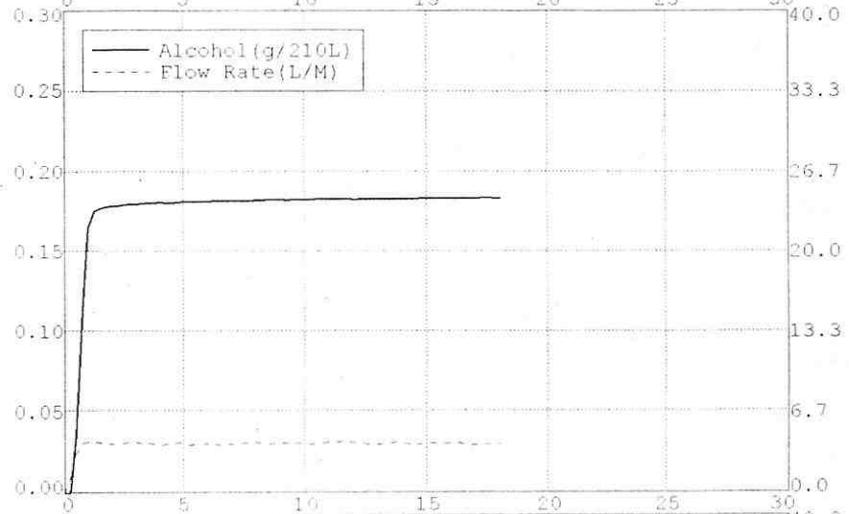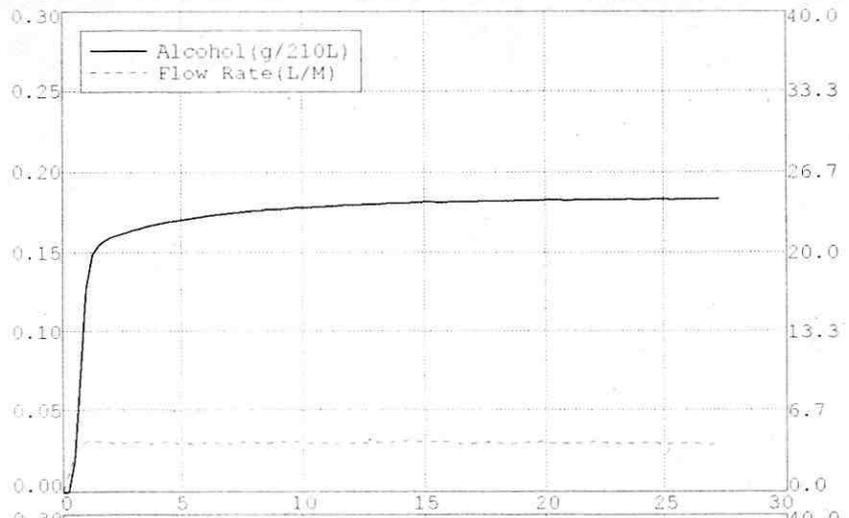

SERVICE AUTHORIZATION FORM
Highway Safety Technology Unit
 80 South Swan Street
 Albany, NY 12210
 Ph: 518-485-7636 / 518-402-0689
 Fax: 518-457-6869

*MS
3/31/21*

THIS FORM IS USED TO AUTHORIZE THE DIVISION OF CRIMINAL JUSTICE SERVICES TO PERFORM SERVICE ON THE INSTRUMENT IDENTIFIED. THIS AUTHORIZATION MUST ACCOMPANY EACH PIECE OF EQUIPMENT WHEN IT IS PRESENTED TO THE EQUIPMENT REPAIR CENTER FOR SERVICE. **PLEASE SIGN AND DATE FORM.**

SECTION I - AGENCY INFORMATION

Name of Agency WARREN COUNTY SHERIFF'S OFFICE		Today's Date 3/28/21
Address 1400 STATE ROUTE 9		City, State, ZIP LAKE GEORGE, NY 12845
Contact Person PATROL SERGEANT C. BENJAMIN GEISLER		Contact Telephone (518) 743-2500
Contact Email ben.geisler@warrencountysheriffny.us		Best Way to Reach You During Appointment Period cell (518) 222-7841

SECTION II - INSTRUMENT INFORMATION

Instrument Manufacturer (Please Circle) NPAS DMT GUTH Applied Concepts (Stalker) Decatur (Genesis) Kustom (Eagle/Falcon) MPH Alco-Sensor Other:		
Model Number DATAMASTER DMT		Instrument Serial Number 105208
Antenna Serial Number (if applicable) Antenna 1 -- / Antenna 2 --		Type of maintenance (check appropriate) <input type="checkbox"/> Calibration Check <input checked="" type="checkbox"/> Repair
Brief Description of Malfunction ATTEMPTED WEEKLY SUPERVISOR TEST. FIRST TEST NEAR COMPLETION CANCELLED DUE TO BLANK ERROR. CHECKED CONNECTIONS AND RAN 2ND SUPERVISOR TEST. TEST RAN TO COMPLETION BUT REFERENCE STANDARD SHOWED 0.00% FOR EACH OF THE THREE TESTS. TOOK ALL TUBES AND CONNECTIONS APART, CHECKED BREATH TUBE FOR DEBRIS, REASSEMBLED AND RAN TEST AGAIN. TEST CANCELLED. INTERFERENCE/ BLANK ERROR. THERE WERE NO CHEMICALS/ SOLVENTS OR ANY TYPES OF SMELL PRESENT. TEST RAN FINE LAST WEEK.		
List all parts, cables and/or accessories being submitted. Tuning forks must accompany all radar units (if applicable). (Please Circle)		
DMT/SIM: DMT SIM Tubes Keyboard Other:		Radar: Control Unit Antenna(s) Antenna Cable(s) Power Cord Forks Other:
I acknowledge I am signing this Service Authorization Form as an act and deed of said agency, organization, or municipality, and that I am duly authorized to sign same for the uses and purposes mentioned herein. PLEASE SIGN AND DATE.		
Signature <i>[Handwritten Signature]</i>		Date 3/28/21

DCJS USE ONLY

Cleaned Sway and plunger. Checked setpoint voltages print and remote operation. Performed calibration/adjustment procedure. Ran subject, technical and diagnostic tests. Verified calibration.