



**CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS
MAINTAINED IN THE REGULAR COURSE OF BUSINESS**

I, **Steven J. Carluccio**, Highway Safety Equipment Technical Supervisor, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NATL PATENT ANALYTICAL SYSTEM, DATAMASTER DMT breath test instrument, serial number 105208, performed on December 06, 2022 by Office of Public Safety employee Martin Schilling, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/ maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance /calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink that reads "Steven J. Carluccio".

Digitally signed under ESRA
by Steven J. Carluccio
on 12/14/2022 10:03 AM

Steven J. Carluccio
Highway Safety Equipment Technical Supervisor
Office of Public Safety

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Warren County Sheriff's Office

Manufacturer: NATL PATENT ANALYTICAL SYSTEM

Model: DATAMASTER DMT

Serial Number: 105208

Date: December 06, 2022

Reference Solution Lot Number : 22120

Reference Solution Standard : 0.10% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.099 %	34.01 degrees centigrade
2	0.098 %	34.02 degrees centigrade
3	0.099 %	34.01 degrees centigrade
4	0.098 %	34.01 degrees centigrade

Reference Solution Lot Number : 22210

Reference Solution Standard : 0.08% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.080 %	34.01 degrees centigrade
2	0.080 %	34.01 degrees centigrade
3	0.080 %	34.01 degrees centigrade
4	0.080 %	34.01 degrees centigrade

Reference Solution Lot Number : 22060

Reference Solution Standard : 0.18% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.183 %	34.01 degrees centigrade
2	0.183 %	34.01 degrees centigrade
3	0.184 %	34.01 degrees centigrade
4	0.184 %	34.01 degrees centigrade

I hereby certify that I have performed any necessary maintenance procedures and calibrated NATL PATENT ANALYTICAL SYSTEM breath test instrument model DATAMASTER DMT, serial number 105208, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.


I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.

Performed by:



Digitally signed under ESRA
by Martin Schilling
on 12/06/2022 08:46 AM

Reviewed by:

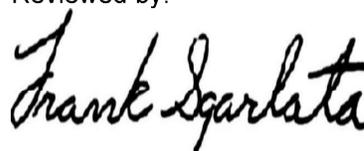

Digitally signed under ESRA
by Frank Sgarlata
on 12/06/2022 11:46 AM

Martin Schilling
Highway Safety Equipment Technician
Breath Analysis Operator Permit #45926

Frank Sgarlata
Breath Analysis Technical Supervisor

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Warren County Sheriff's Office
Manufacturer: NATL PATENT ANALYTICAL SYSTEM
Model: DATAMASTER DMT
Serial Number: 105208
Date: December 06, 2022

- 1. General appearance and condition of this device -----: **BLANK ERROR**

- 2. Check controls and indicators -----: **OK**

- 3. Check breath flow system -----: **OK**

- 4. Check printer operation -----: **OK**

- 5. System cycles through all modes -----: **OK**

- 6. Record any repairs made to this instrument and list services provided : **CLEANED 5-WAY VALVE. INSPECTED INSTRUMENT, CHECKED SETUP VOLTAGES PRINT AND REMOTE OPERATION. PERFORMED CALIBRATION/ADJUSTMENT PROCEDURE, RAN SUBJECT, TECHNICIAN AND DIAGNOSTIC TESTS, VERIFIED CALIBRATION.**



Performed by:

Digitally signed under ESRA
by Martin Schilling
on 12/06/2022 08:46 AM

**Martin Schilling
Highway Safety Equipment Technician
Breath Analysis Operator Permit #45926**

Reviewed by:

Digitally signed under ESRA
by Frank Sgarlata
on 12/06/2022 11:46 AM

**Frank Sgarlata
Breath Analysis Technical Supervisor**

TECHNICIAN TEST

WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208





Date: 12/06/2022

OPERATOR NAME:
MARTIN J SCHILLING
Permit #: 45926
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 22210

Nominal = 0.080 g/210L

BLANK TEST	0.000	07:51
INTERNAL STANDARD	VERIFIED	07:51
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.080	07:52
BLANK TEST	0.000	07:53
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.080	07:53
BLANK TEST	0.000	07:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.080	07:54
BLANK TEST	0.000	07:55
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.080	07:55
BLANK TEST	0.000	07:56

Average = 0.0800
Std Dev = 0.0000

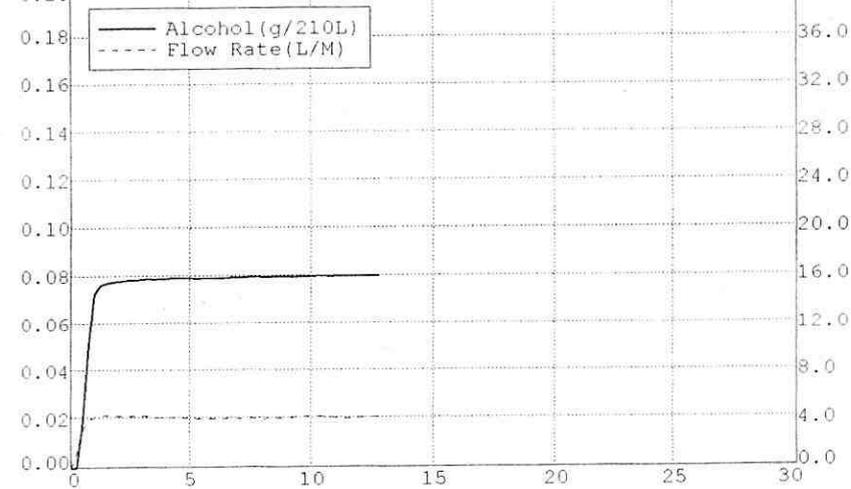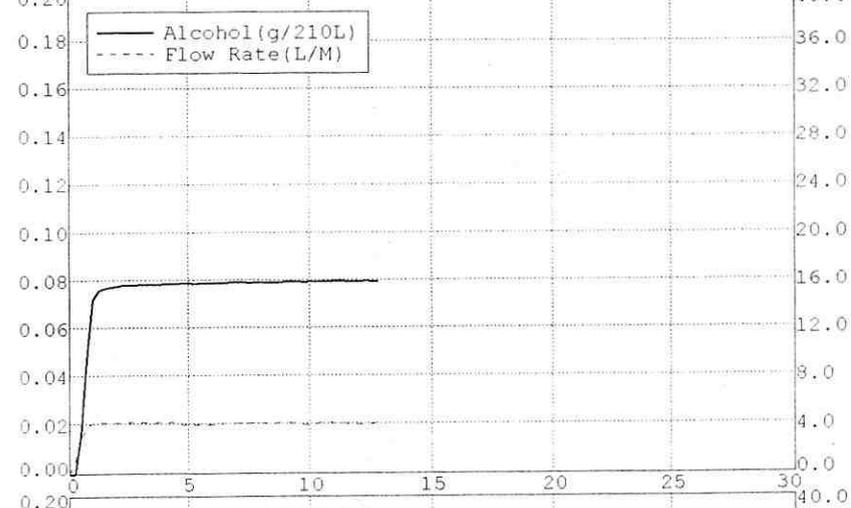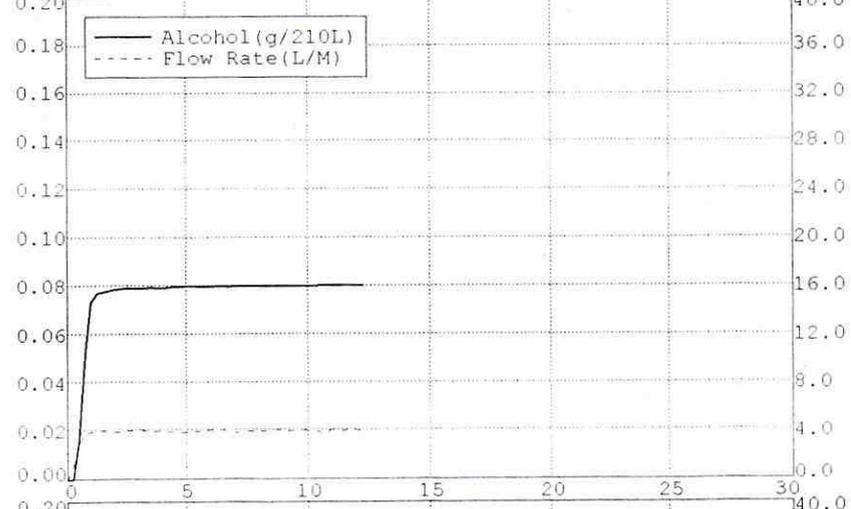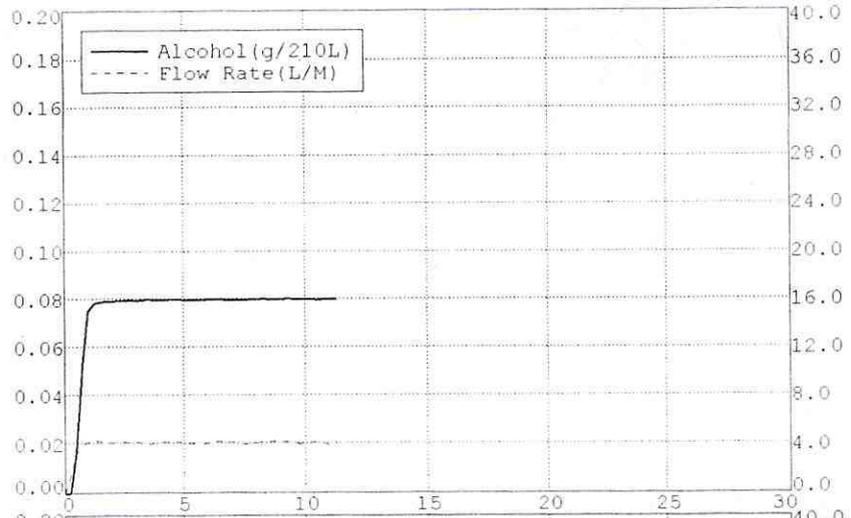

TECHNICIAN TEST

WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208


Date: 12/06/2022

OPERATOR NAME:
MARTIN J SCHILLING
Permit #: 45926
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 22120

Nominal = 0.100 g/210L

BLANK TEST	0.000	07:44
INTERNAL STANDARD	VERIFIED	07:44
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.099	07:45
BLANK TEST	0.000	07:46
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.098	07:46
BLANK TEST	0.000	07:47
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.099	07:47
BLANK TEST	0.000	07:48
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.098	07:48
BLANK TEST	0.000	07:49

Average = 0.0985
Std Dev = 0.0006

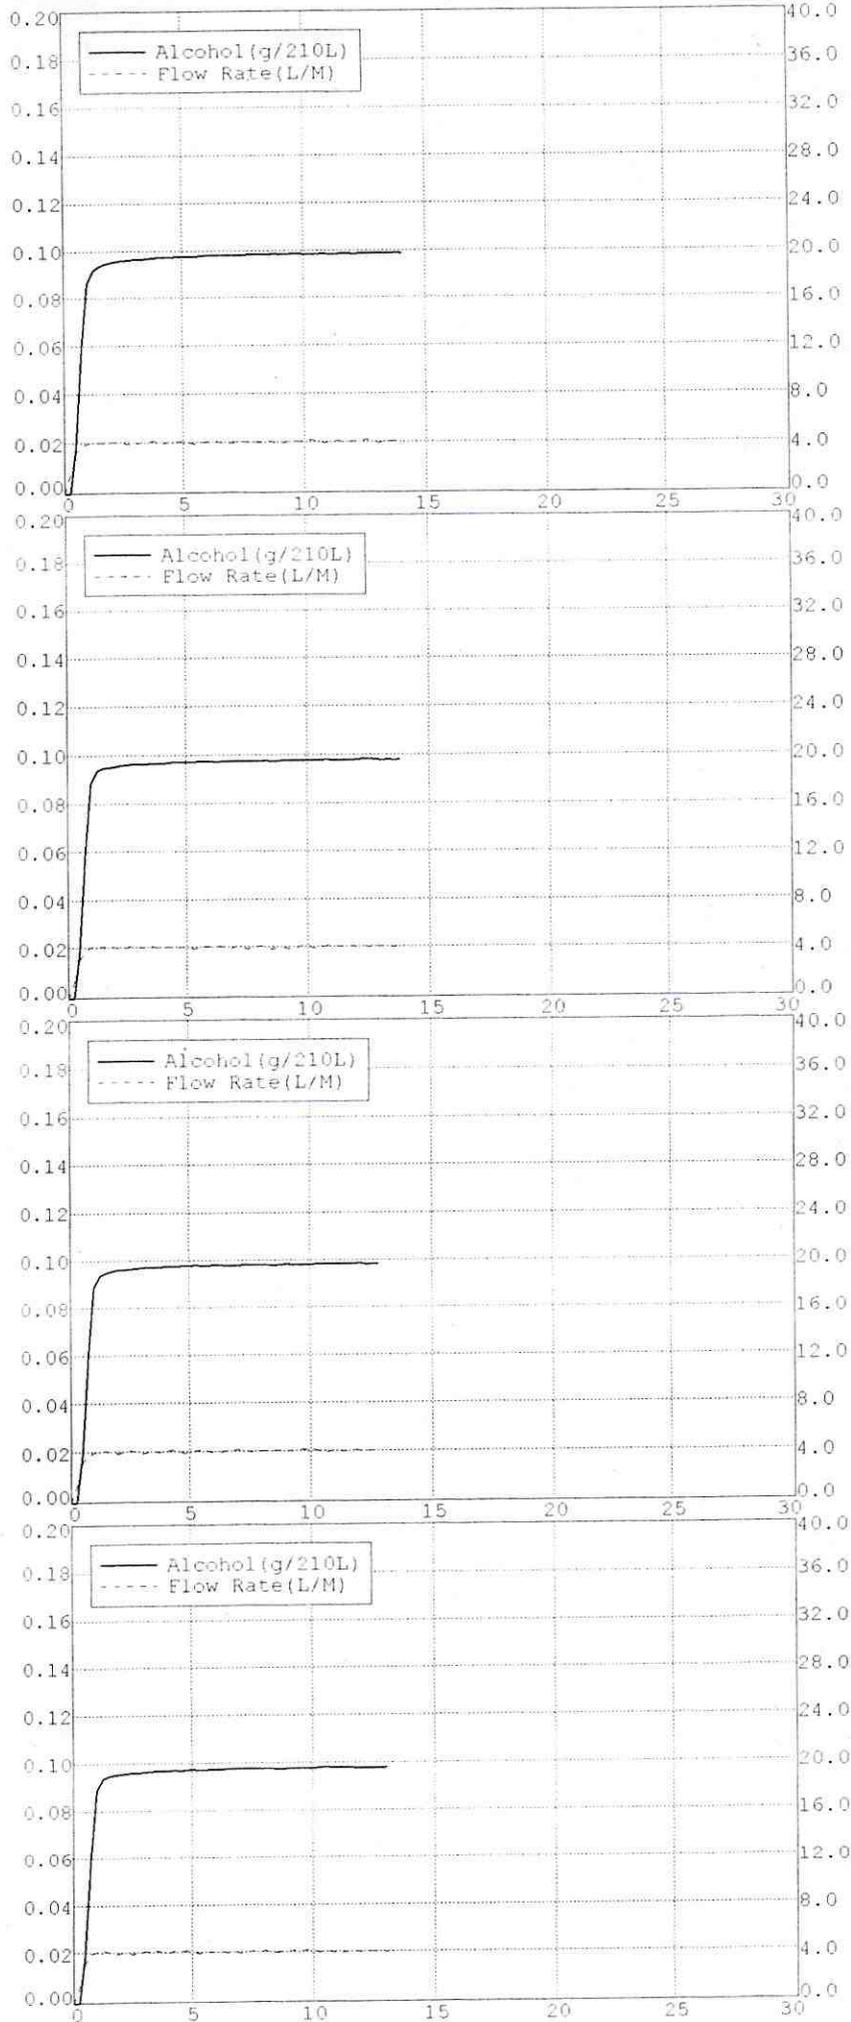

TECHNICIAN TEST

WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208


Date: 12/06/2022

OPERATOR NAME:
MARTIN J SCHILLING
Permit #: 45926
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 22060

Nominal = 0.180 g/210L

BLANK TEST	0.000	08:04
INTERNAL STANDARD	VERIFIED	08:04
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.183	08:04
BLANK TEST	0.000	08:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.183	08:06
BLANK TEST	0.000	08:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.184	08:07
BLANK TEST	0.000	08:08
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.184	08:08
BLANK TEST	0.000	08:09

Average = 0.1835
Std Dev = 0.0006

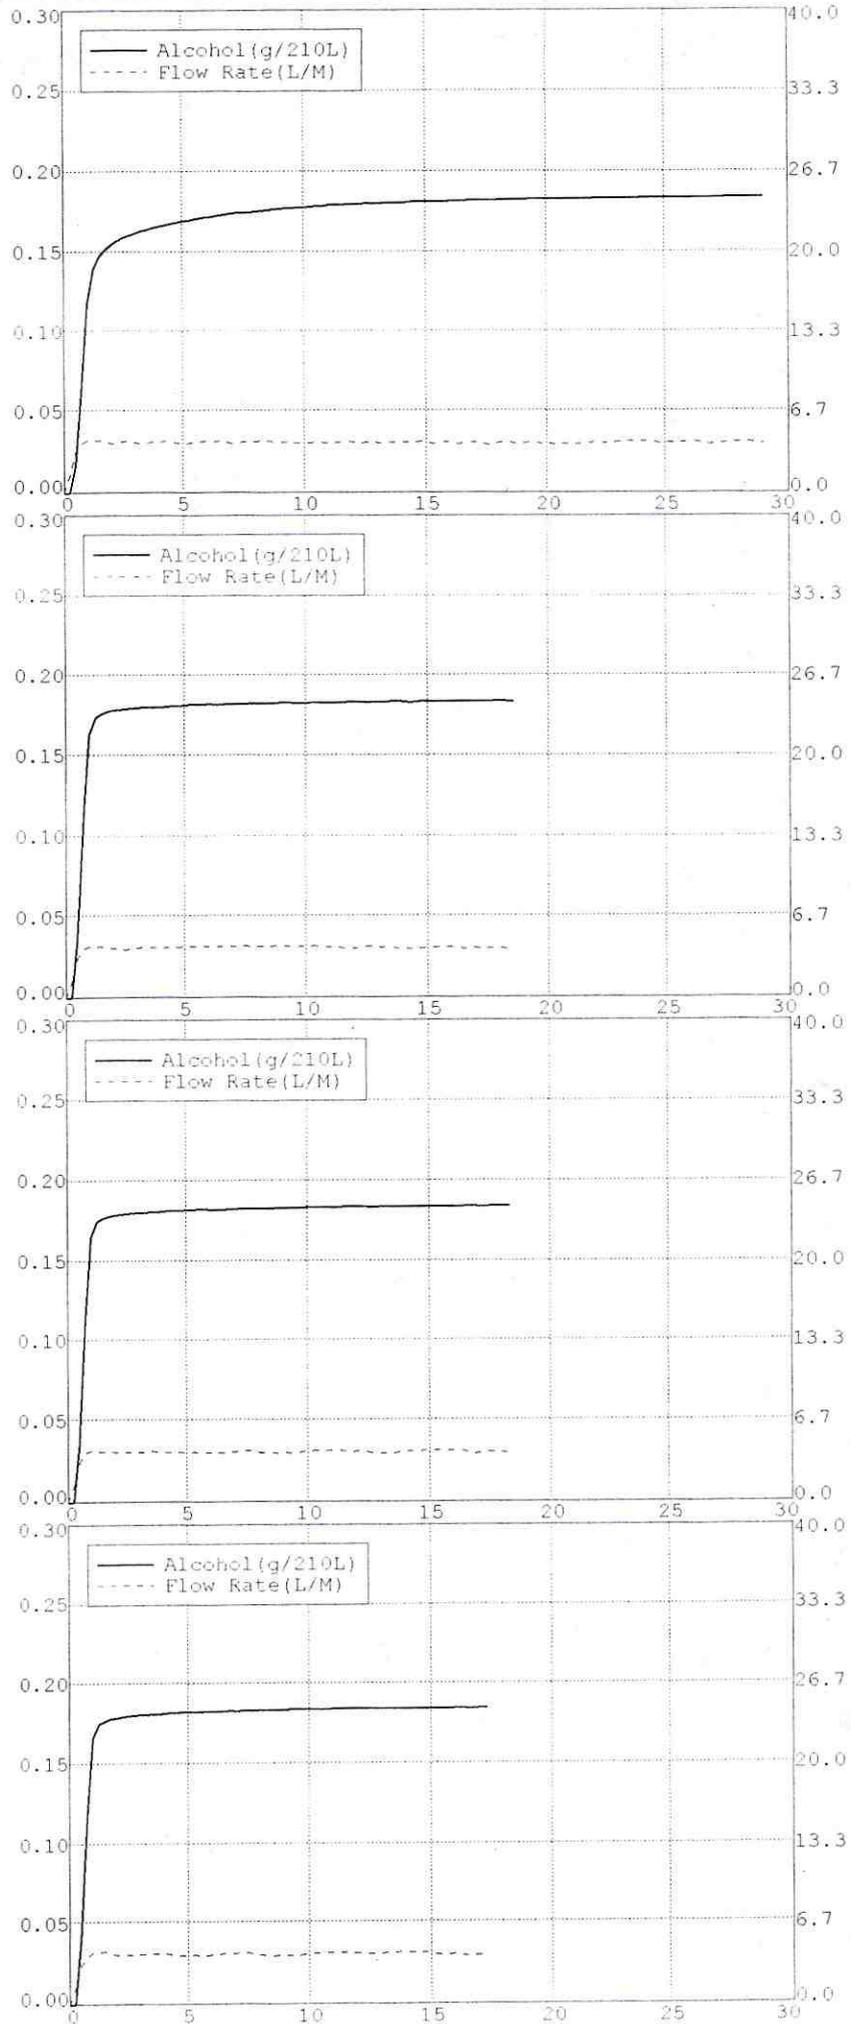

SERVICE AUTHORIZATION FORM
Highway Safety Technology Unit
80 South Swan Street
Albany, NY 12210
Ph: 518-485-7636 / 518-402-0689
Fax: 518-457-6869

*py
12/16/22*

THIS FORM IS USED TO AUTHORIZE THE DIVISION OF CRIMINAL JUSTICE SERVICES TO PERFORM SERVICE ON THE INSTRUMENT IDENTIFIED. THIS AUTHORIZATION MUST ACCOMPANY EACH PIECE OF EQUIPMENT WHEN IT IS PRESENTED TO THE EQUIPMENT REPAIR CENTER FOR SERVICE. **PLEASE SIGN AND DATE FORM.**

SECTION I - AGENCY INFORMATION

Name of Agency WARREN COUNTY SHERIFF'S OFFICE		Today's Date 12/02/2022
Address 1400 U.S. 9		City, State, ZIP LAKE GEORGE, NY 12845
Contact Person SGT C.B. GEISLER		Contact Telephone 518-743-2500 x1
Contact Email Ben.Geisler@WarrenCountySheriffNY.us		Best Way to Reach You During Appointment Period 518-743-2500 x1

SECTION II - INSTRUMENT INFORMATION

Instrument Manufacturer (Please Circle) NPAS DMT GUTH Applied Concepts (Stalker) Decatur (Genesis) Kustom (Eagle/Falcon) MPH Alco-Sensor Other:		
Model Number DATAMASTER DMT		Instrument Serial Number 105208
Antenna Serial Number (if applicable) Antenna 1 -- / Antenna 2 --		Type of maintenance (check appropriate) <input checked="" type="checkbox"/> Calibration Check <input checked="" type="checkbox"/> Repair
Brief Description of Malfunction 1) 12/01/2022 - ALL THREE REFERENCE STANDARDS ON SUPERVISOR TEST SHOWED ZERO WITH NO SLOPE DETECTION, POSSIBLY CAUSED BY A STICKY 5-WAY VALVE ACCORDING TO A PHONE CALL WITH A TECH. 2) 12/02/2022 - UNEXPLAINABLE BLANK ERROR ON SUPERVISOR TEST.		
List all parts, cables and/or accessories being submitted. Tuning forks must accompany all radar units (if applicable). (Please Circle)		
DMT/SIM: DMT 105208 Keyboard 1	SIM MP4824 Other: x2 power cords, x1 simulator data	Radar: Control Unit Antenna(s) Antenna Cable(s) Power Cord Forks Other:
I acknowledge I am signing this Service Authorization Form as an act and deed of said agency, organization, or municipality, and that I am duly authorized to sign same for the uses and purposes mentioned herein. PLEASE SIGN AND DATE.		
Signature <i>[Signature]</i>		Date 12/02/2022

DCJS USE ONLY

Cleared Survey online. I inspected instrument, checked voltage, ground and master operation. Performed calibration/adjustment procedure. Ran subject, technician and designated tests. Verified calibration.