

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106206

Date: 01/27/2008

Operator Name: RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 07250

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:25
INTERNAL STANDARD	VERIFIED	18:25
REFERENCE STANDARD TEMP	34.0c	
REFERENCE STANDARD	0.09	18:26
REFERENCE STANDARD TEMP	34.0c	
REFERENCE STANDARD	0.09	18:27
REFERENCE STANDARD TEMP	34.0c	
REFERENCE STANDARD	0.09	18:28
BLANK TEST	0.00	18:28

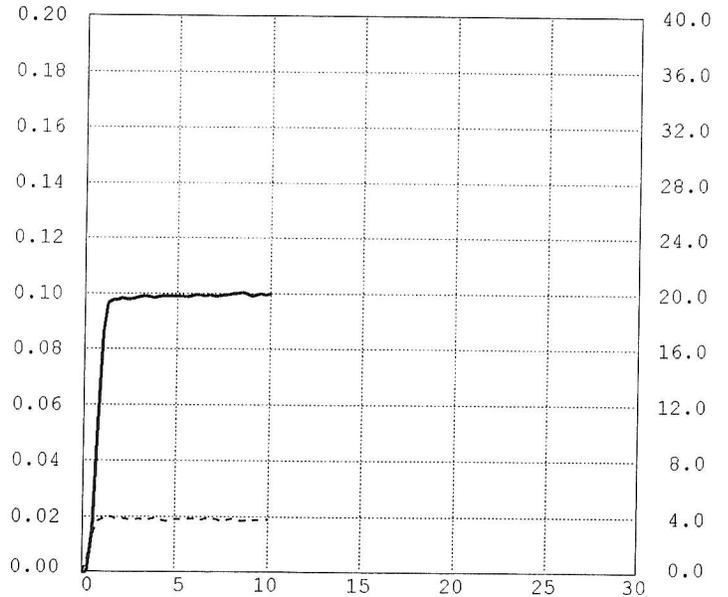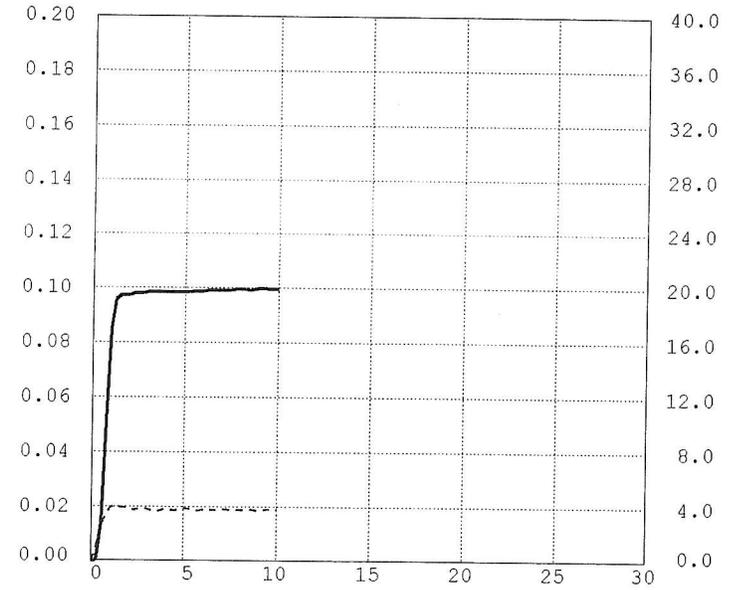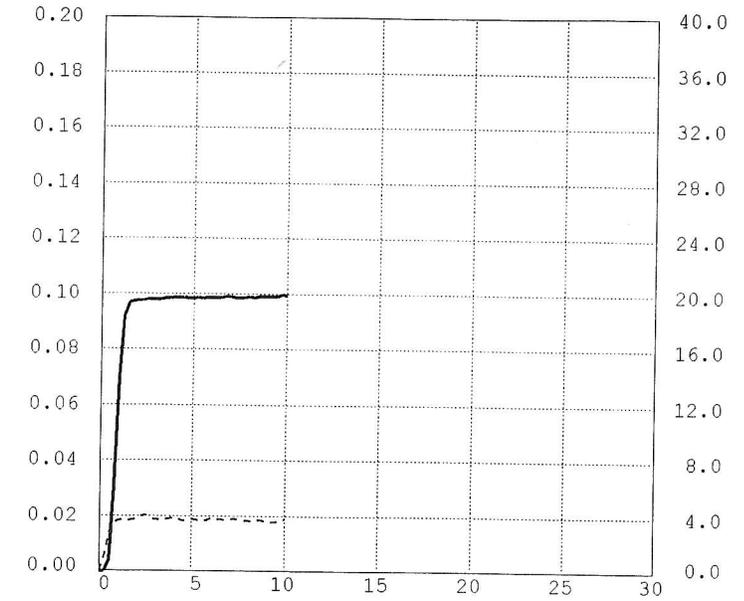

SCA Range 7, Bartlett 1/27/08