

SOLUTION CHANGE





-----  
 WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 106206  
 -----

Date: 12/02/2007

Operator Name: RALPH J BARTLETT  
 Permit #: 26222  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 07250

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:58
INTERNAL STANDARD	VERIFIED	03:58
REFERENCE STANDARD TEMP	34.0c	
REFERENCE STANDARD	0.09	03:58
REFERENCE STANDARD TEMP	34.0c	
REFERENCE STANDARD	0.09	03:59
REFERENCE STANDARD TEMP	34.0c	
REFERENCE STANDARD	0.09	04:00
BLANK TEST	0.00	04:01

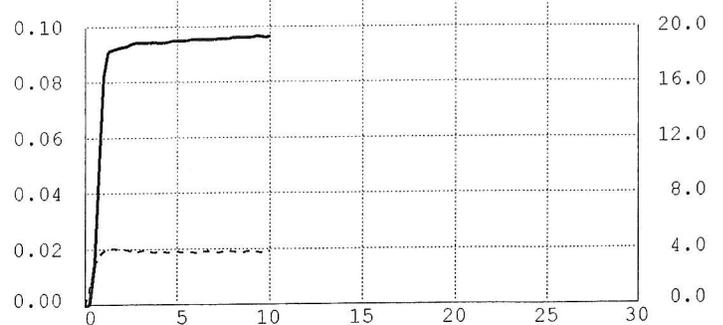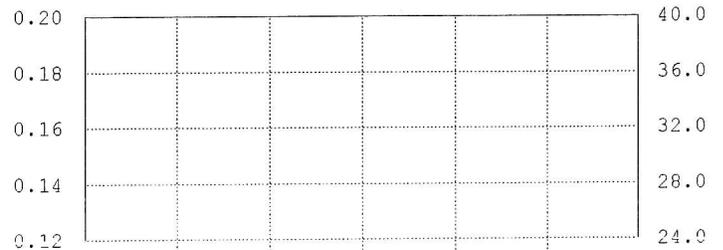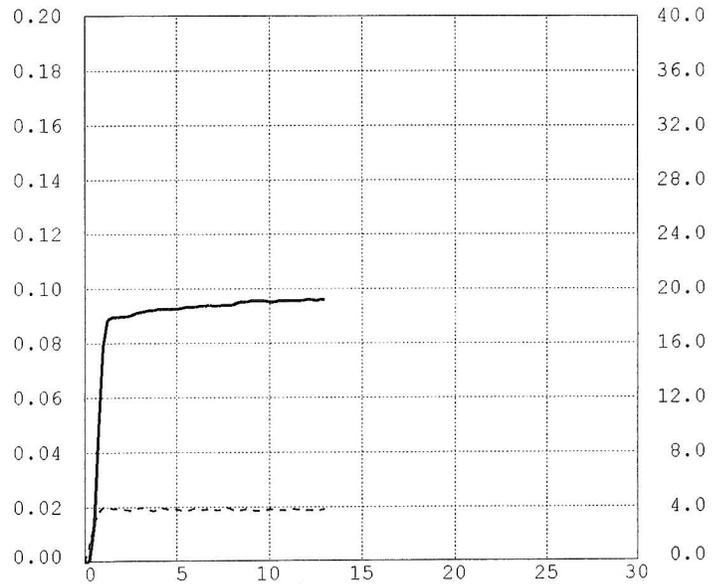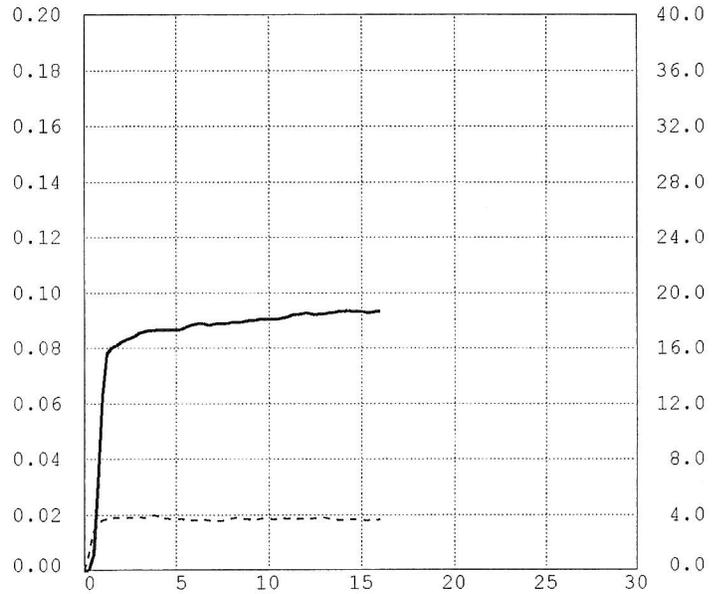

SG5 High Purity #162 12/2/07