

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106206

Date: 01/08/2008

Operator Name: RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN COUNTY SHERIFF'S OFFICE  
Reference Standard #: 07250

Nominal = 0.10 g/210L

|                         |          |       |
|-------------------------|----------|-------|
| BLANK TEST              | 0.00     | 02:32 |
| INTERNAL STANDARD       | VERIFIED | 02:32 |
| REFERENCE STANDARD TEMP | 34.0c    |       |
| REFERENCE STANDARD      | 0.10     | 02:32 |
| REFERENCE STANDARD TEMP | 34.0c    |       |
| REFERENCE STANDARD      | 0.10     | 02:33 |
| REFERENCE STANDARD TEMP | 34.0c    |       |
| REFERENCE STANDARD      | 0.10     | 02:34 |
| BLANK TEST              | 0.00     | 02:35 |

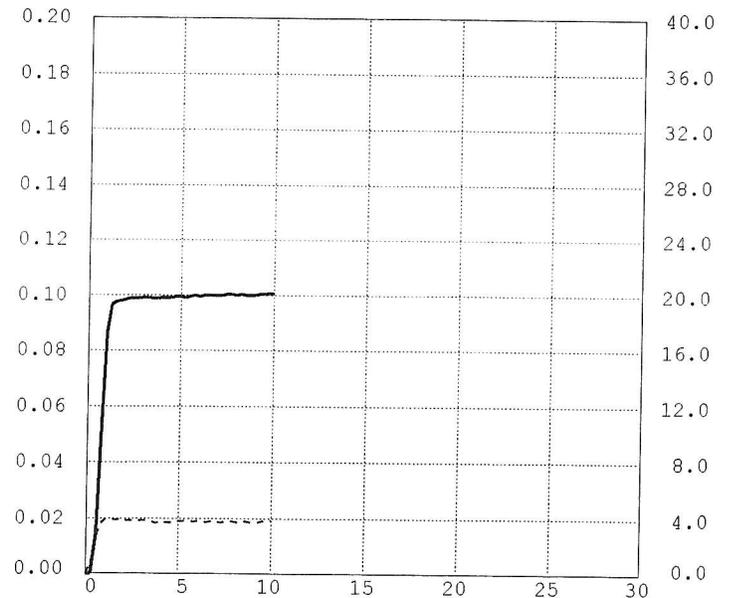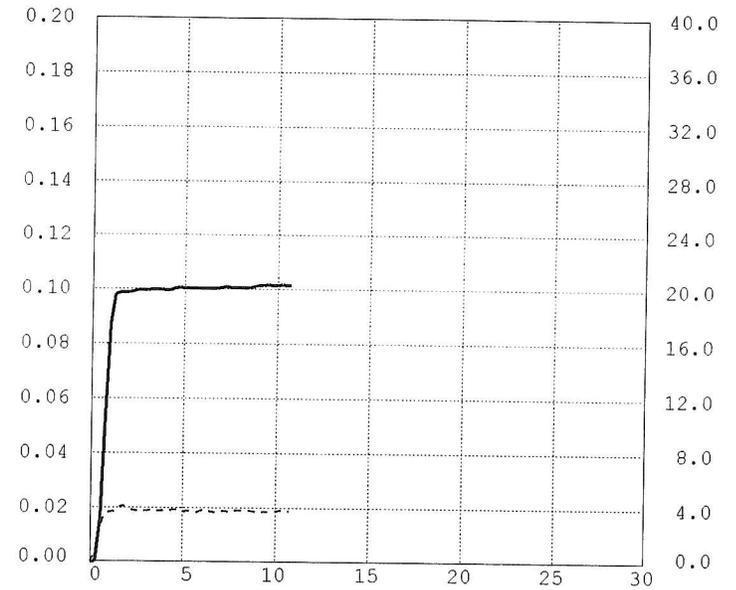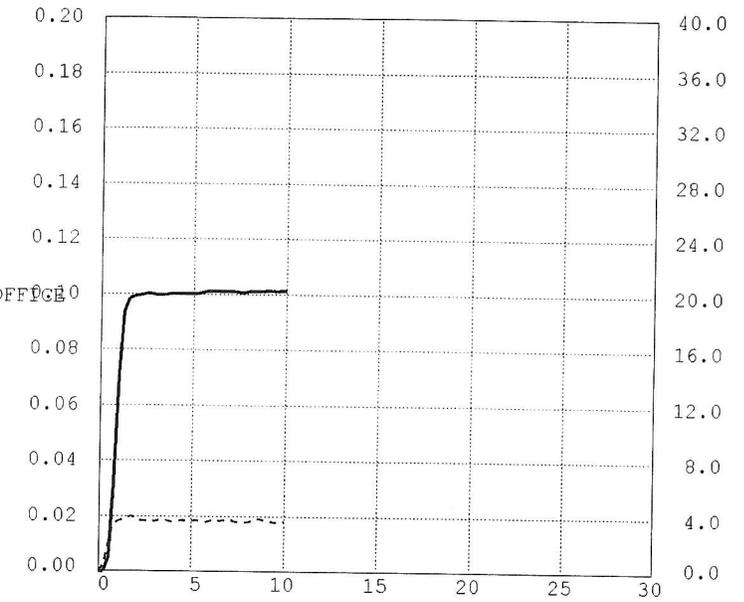

505 *Ralph Bartlett* 1/8/08