

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106206

Date: 03/14/2008

Operator Name: CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 07300

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 13:57 |
| INTERNAL STANDARD | VERIFIED | 13:57 |
| REFERENCE STANDARD TEMP | 34.0c | |
| REFERENCE STANDARD | 0.09 | 13:57 |
| REFERENCE STANDARD TEMP | 34.0c | |
| REFERENCE STANDARD | 0.09 | 13:58 |
| REFERENCE STANDARD TEMP | 34.0c | |
| REFERENCE STANDARD | 0.09 | 14:00 |
| BLANK TEST | 0.00 | 14:01 |

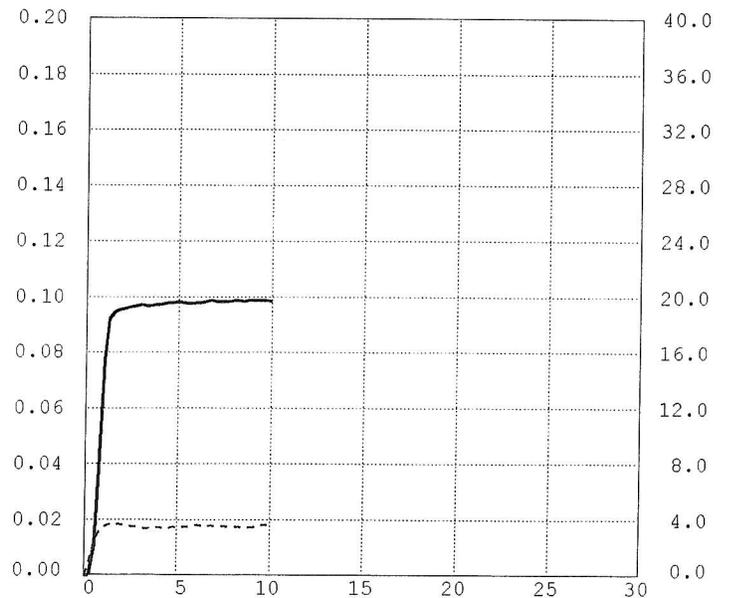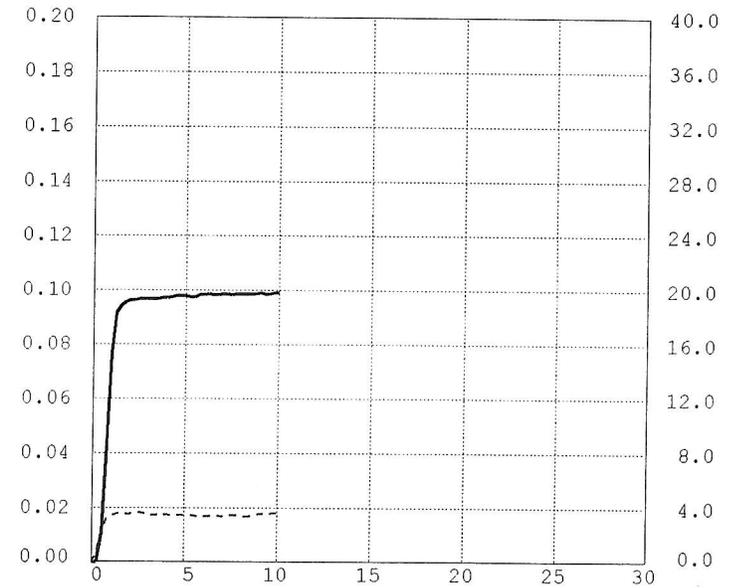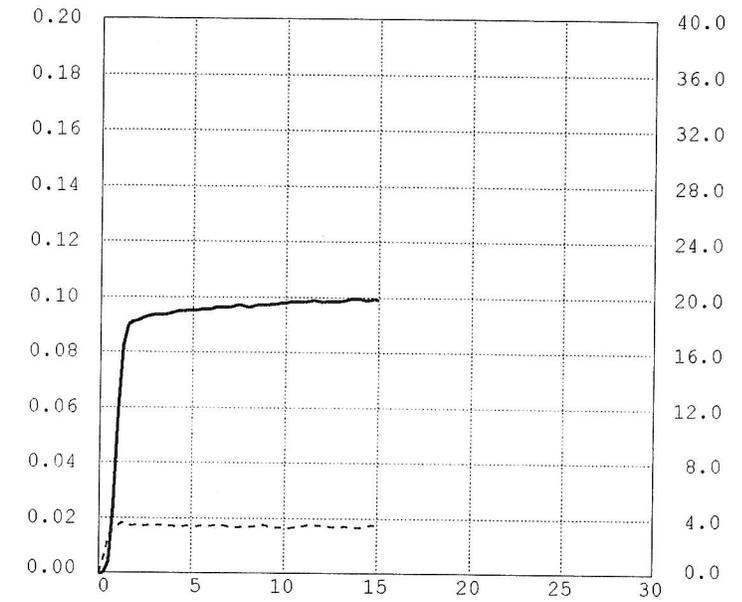

Charles B. Geisler #248
3/14/08