

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106206

Date: 11/23/2008

Operator Name: CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 08220

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:30
INTERNAL STANDARD	VERIFIED	07:30
REFERENCE STANDARD TEMP	34.0c	
REFERENCE STANDARD	0.09	07:30
REFERENCE STANDARD TEMP	34.0c	
REFERENCE STANDARD	0.09	07:31
REFERENCE STANDARD TEMP	34.0c	
REFERENCE STANDARD	0.09	07:32
BLANK TEST	0.00	07:33

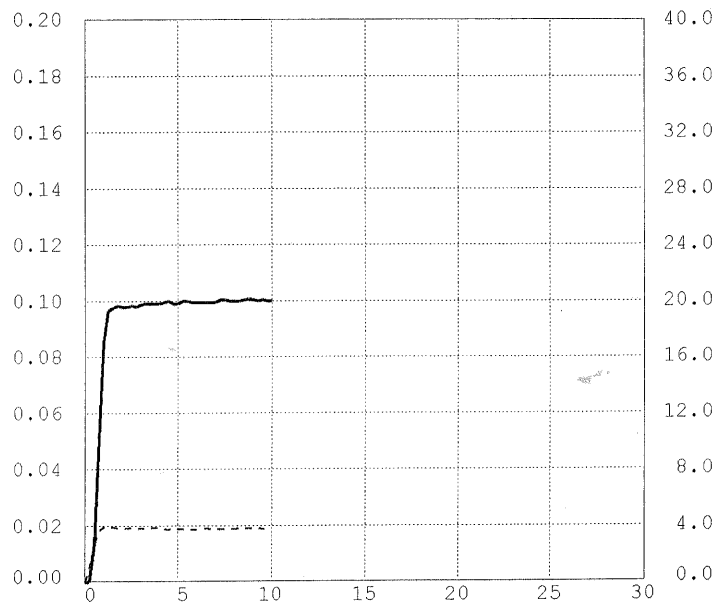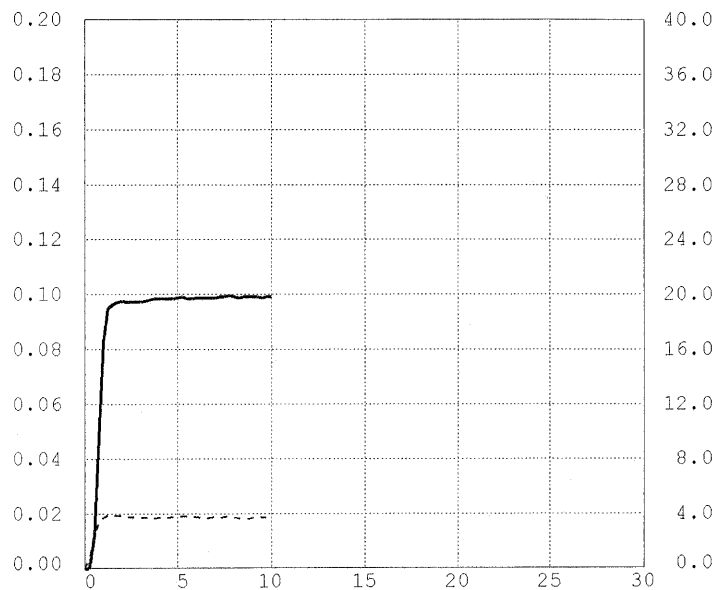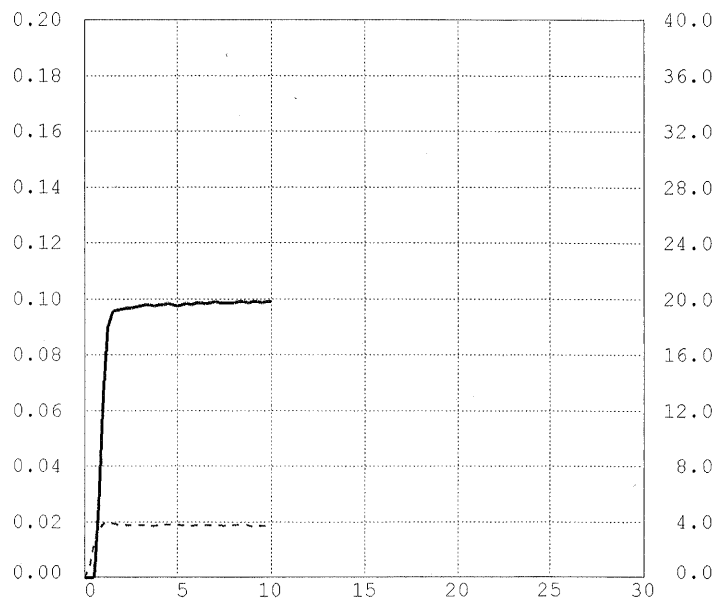

[Handwritten signature]