

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106206

Date: 11/26/2008

Operator Name: CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 08220

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:34
INTERNAL STANDARD	VERIFIED	18:34
REFERENCE STANDARD TEMP	34.0c	
REFERENCE STANDARD	0.10	18:35
REFERENCE STANDARD TEMP	34.0c	
REFERENCE STANDARD	0.09	18:36
REFERENCE STANDARD TEMP	34.0c	
REFERENCE STANDARD	0.09	18:37
BLANK TEST	0.00	18:37

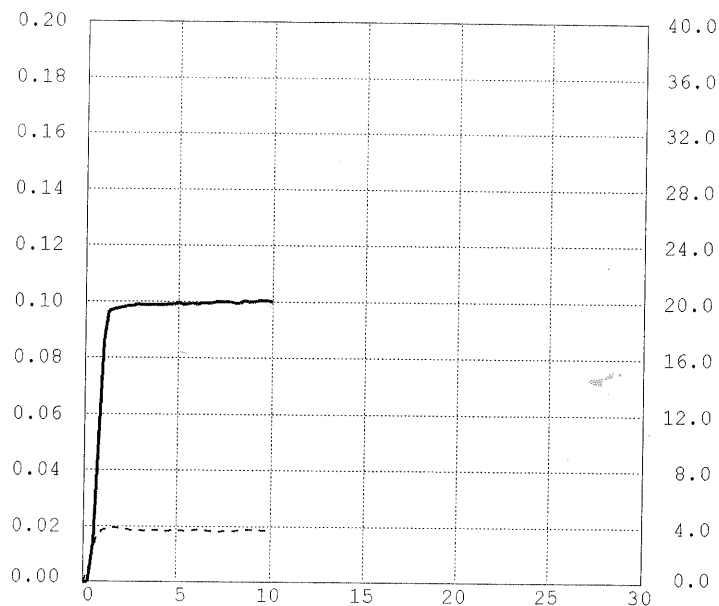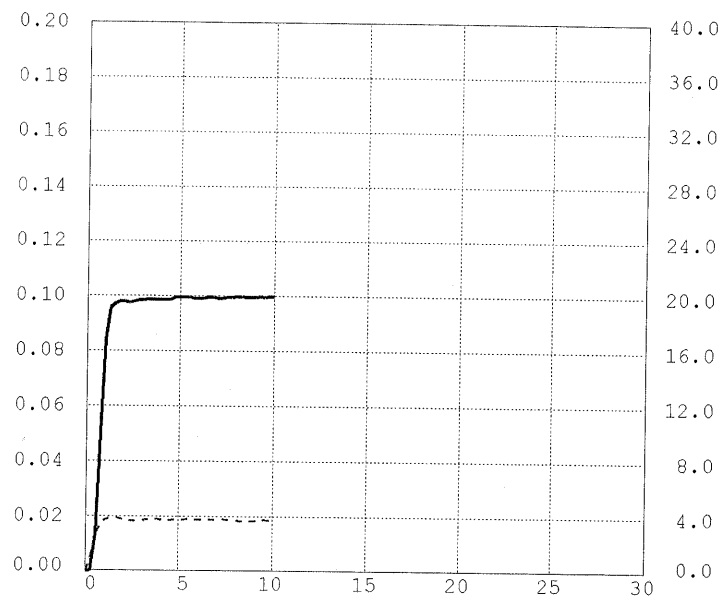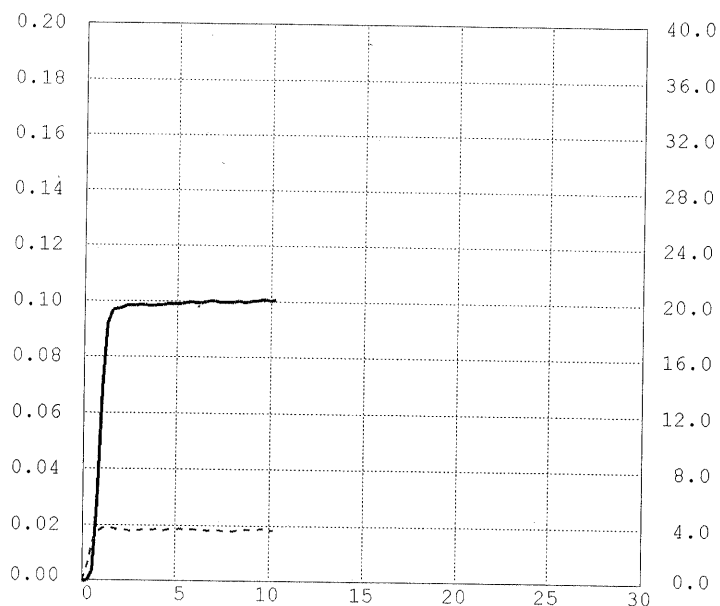

Charles B. Geisler 7248