

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106206

Date: 06/24/2009

Operator Name: RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 09060

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:44
INTERNAL STANDARD	VERIFIED	01:44
REFERENCE STANDARD TEMP	34.0c	
REFERENCE STANDARD	0.09	01:44
REFERENCE STANDARD TEMP	34.0c	
REFERENCE STANDARD	0.09	01:45
REFERENCE STANDARD TEMP	34.0c	
REFERENCE STANDARD	0.09	01:46
BLANK TEST	0.00	01:47

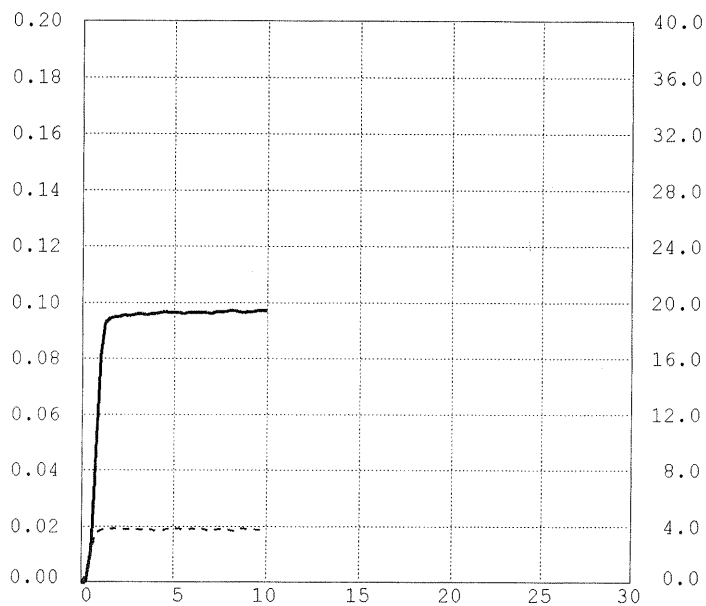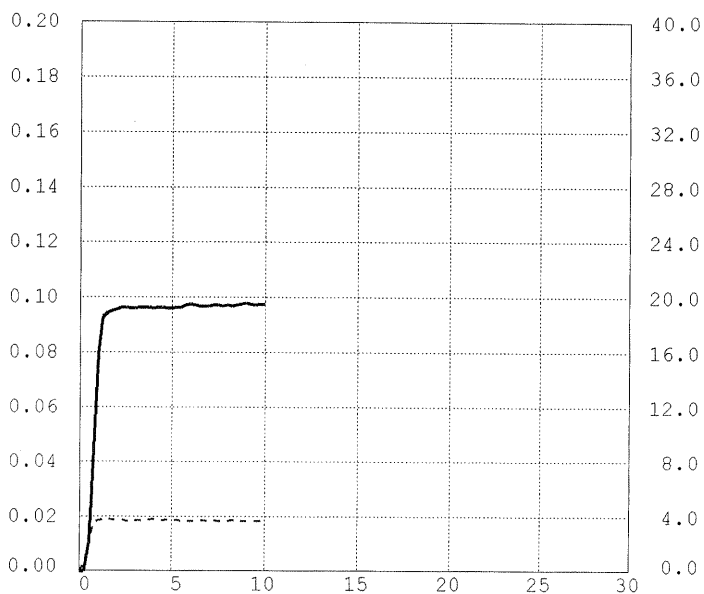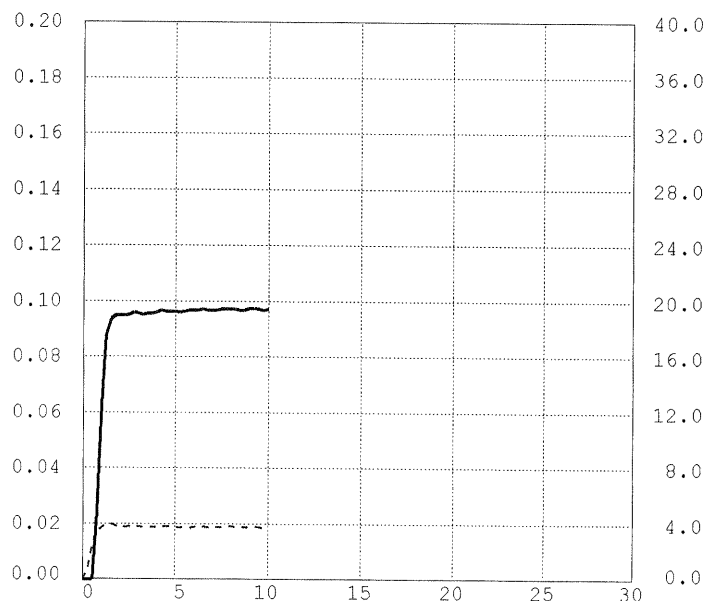

SET Ralph Bartlett 6/24/09