

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106206

Date: 05/08/2010

Operator Name: CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 10010

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:50
INTERNAL STANDARD	VERIFIED	11:51
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	11:51
BLANK TEST	0.00	11:52
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	11:52
BLANK TEST	0.00	11:53
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:53
BLANK TEST	0.00	11:54

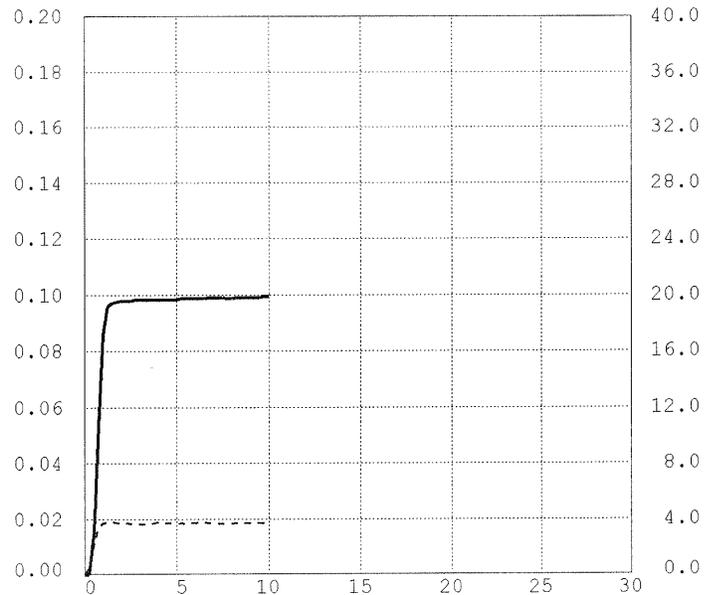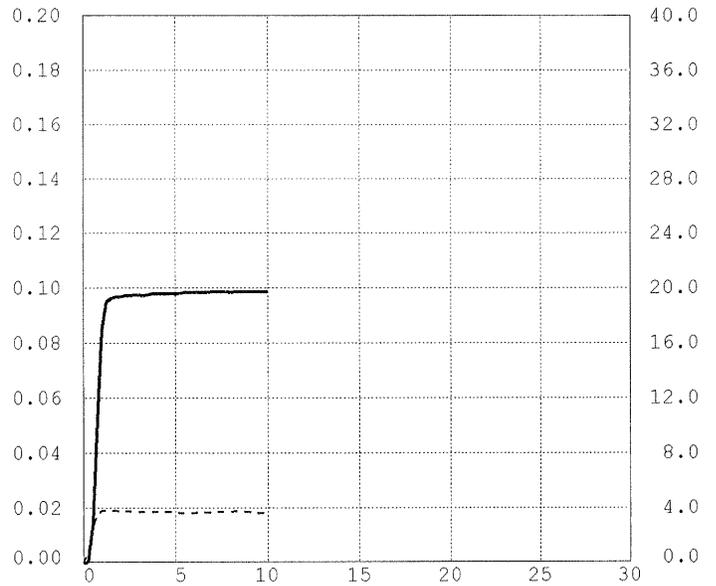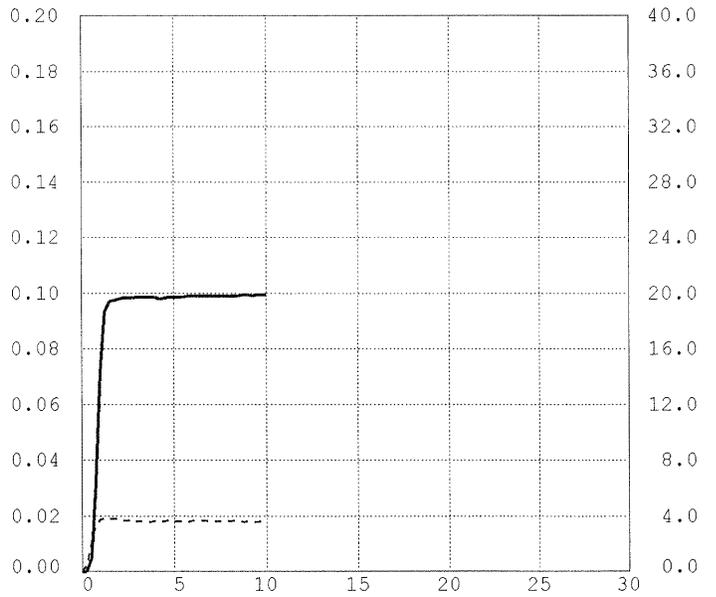

for Charles B. Geisler