

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106206

Date: 06/12/2010

Operator Name: CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 10060

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:48
INTERNAL STANDARD	VERIFIED	15:48
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	15:48
BLANK TEST	0.00	15:49
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:49
BLANK TEST	0.00	15:50
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:50
BLANK TEST	0.00	15:51

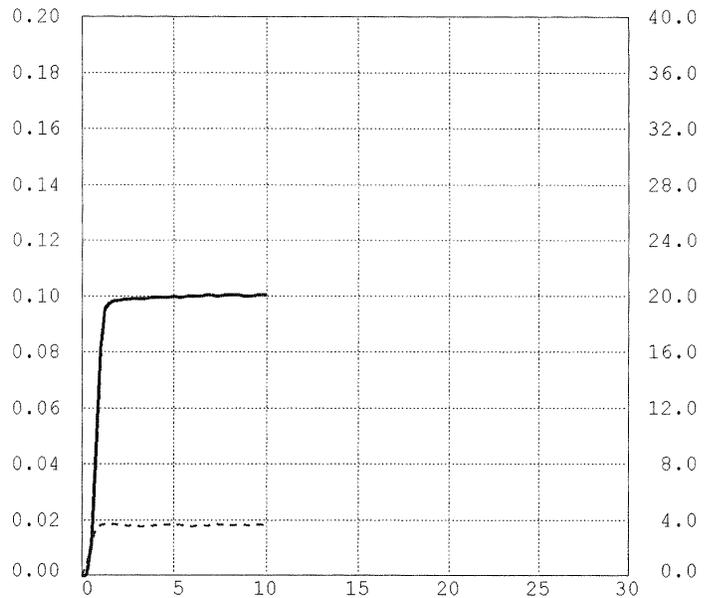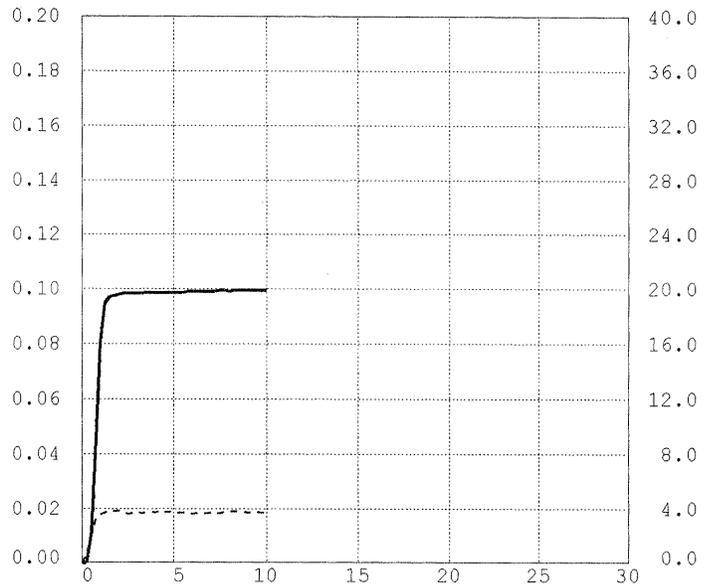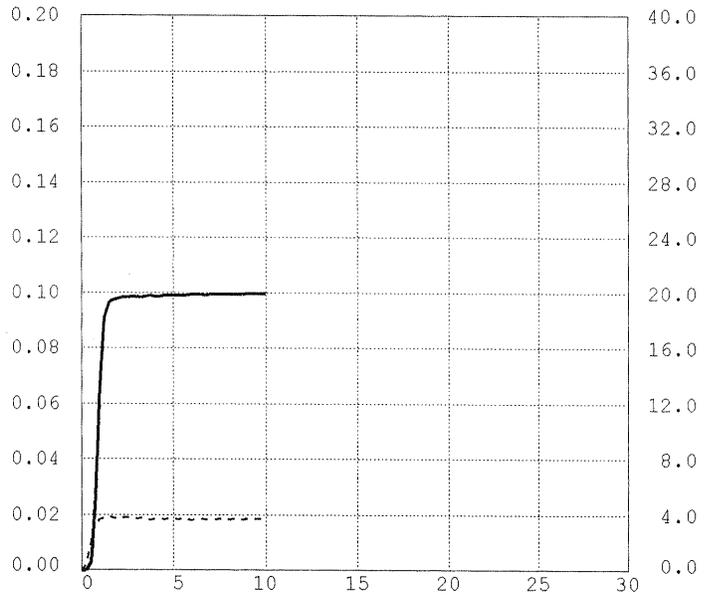

Charles B. Geisler #748 6/12/10 1554