

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106206

Date: 07/27/2010

Operator Name: CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 10060

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:50
INTERNAL STANDARD	VERIFIED	14:50
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	14:50
BLANK TEST	0.00	14:51
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	14:51
BLANK TEST	0.00	14:52
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:52
BLANK TEST	0.00	14:53

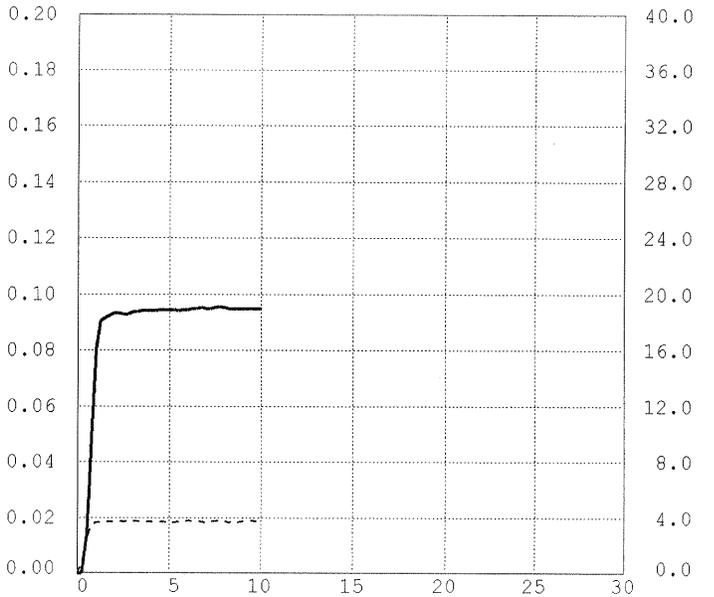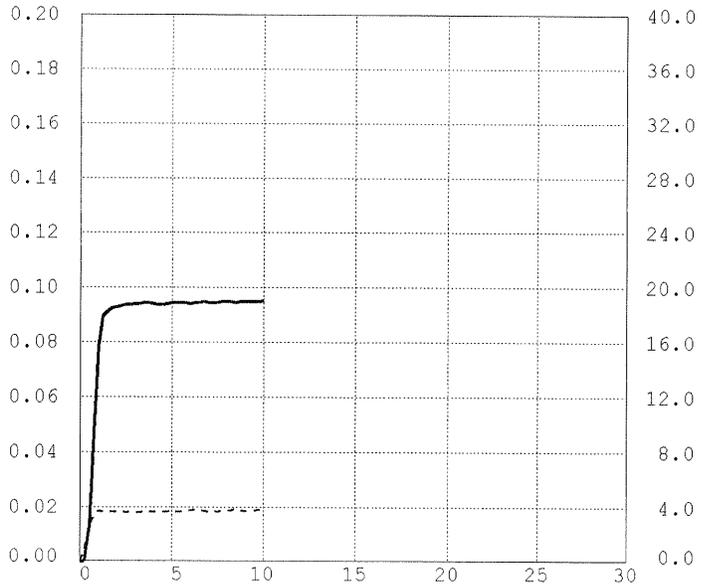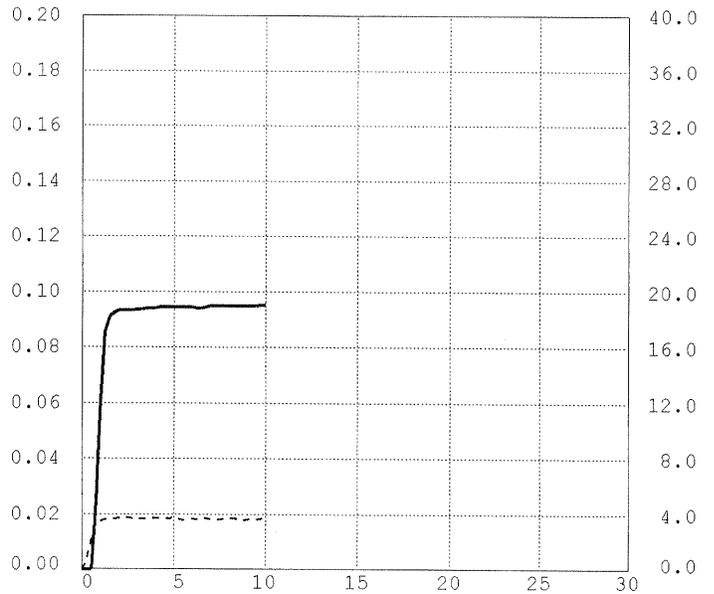

Handwritten signature and notes:
#248 7/27/10 1454