

SUPERVISOR TEST




 WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 106206

Date: 11/09/2011

Operator Name: CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 11140

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:23
INTERNAL STANDARD	VERIFIED	15:23
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	15:24
BLANK TEST	0.00	15:25
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	15:25
BLANK TEST	0.00	15:26
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	15:26
BLANK TEST	0.00	15:27

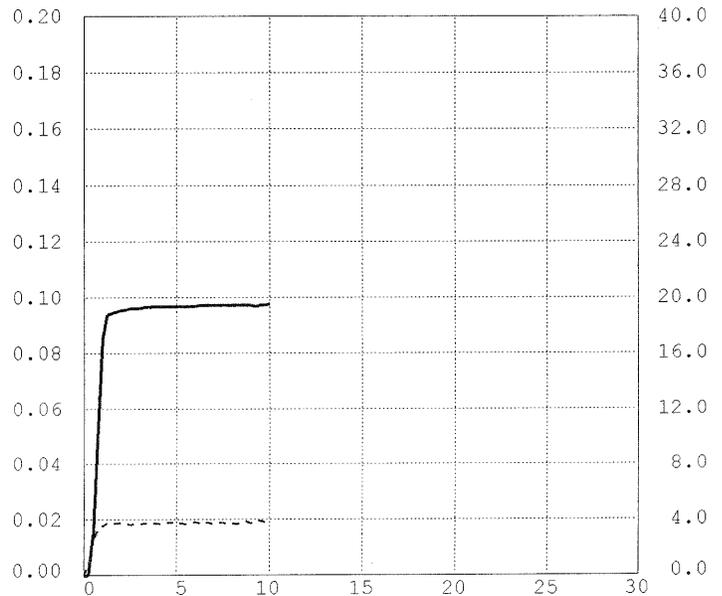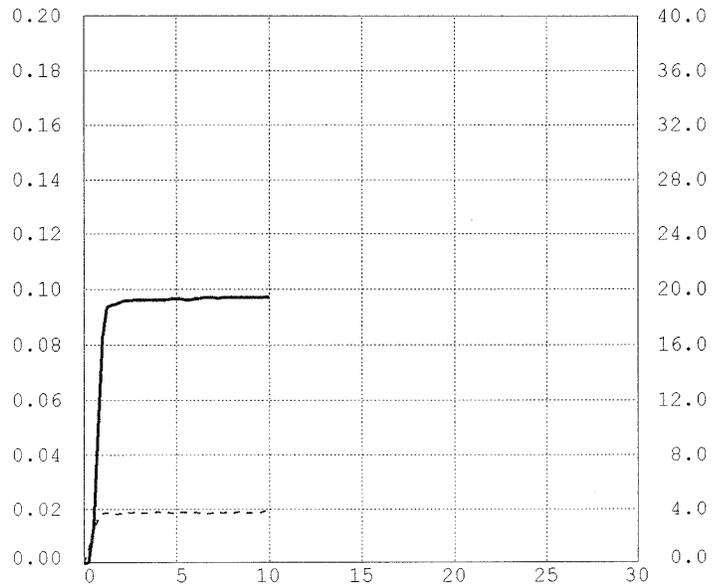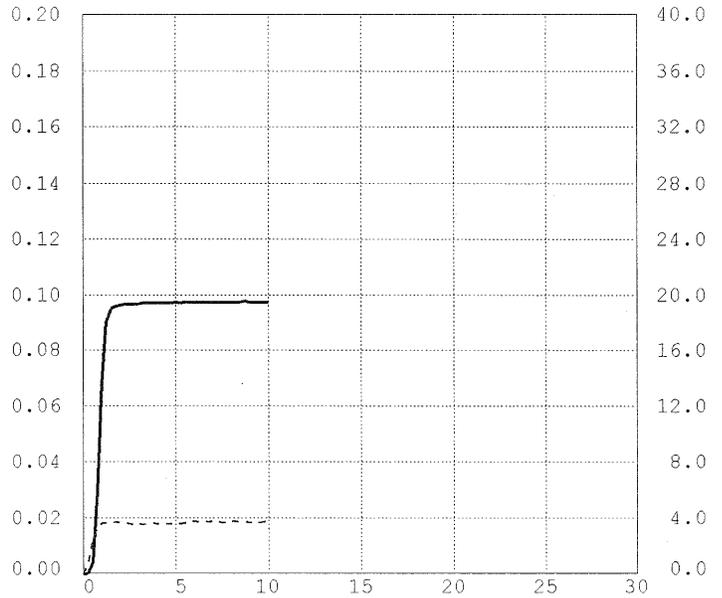

Charles B. Geisler #248 11/09/11 15:27
 HMG