

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106206

Date: 11/23/2011

Operator Name: CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 11140

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 08:34 |
| INTERNAL STANDARD | VERIFIED | 08:34 |
| REFERENCE STANDARD TEMP | 33.99c | |
| REFERENCE STANDARD | 0.09 | 08:34 |
| BLANK TEST | 0.00 | 08:35 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 08:35 |
| BLANK TEST | 0.00 | 08:36 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 08:37 |
| BLANK TEST | 0.00 | 08:37 |

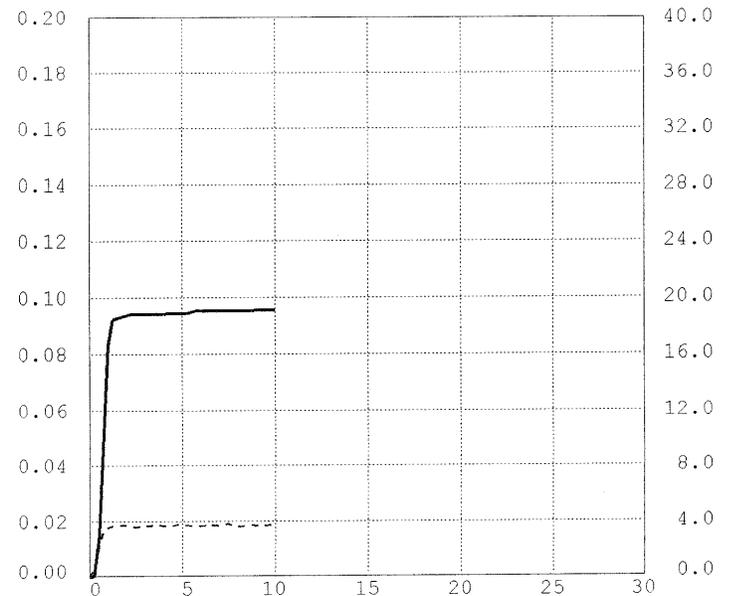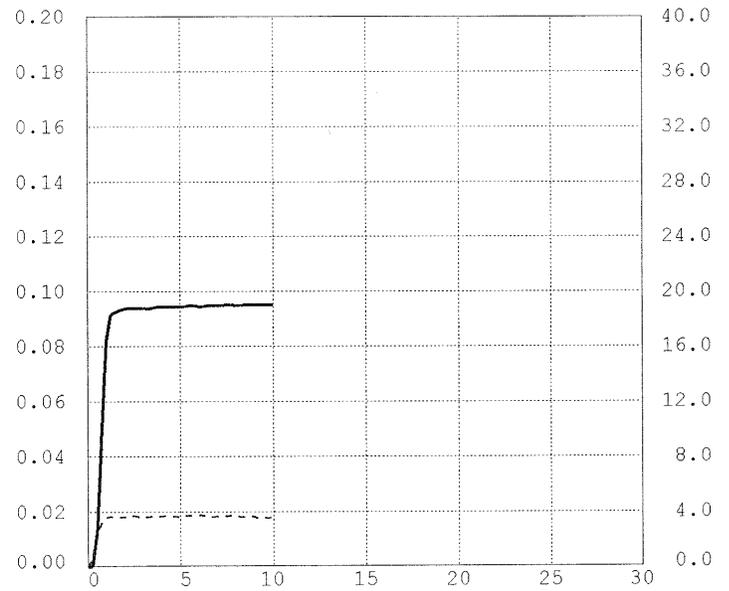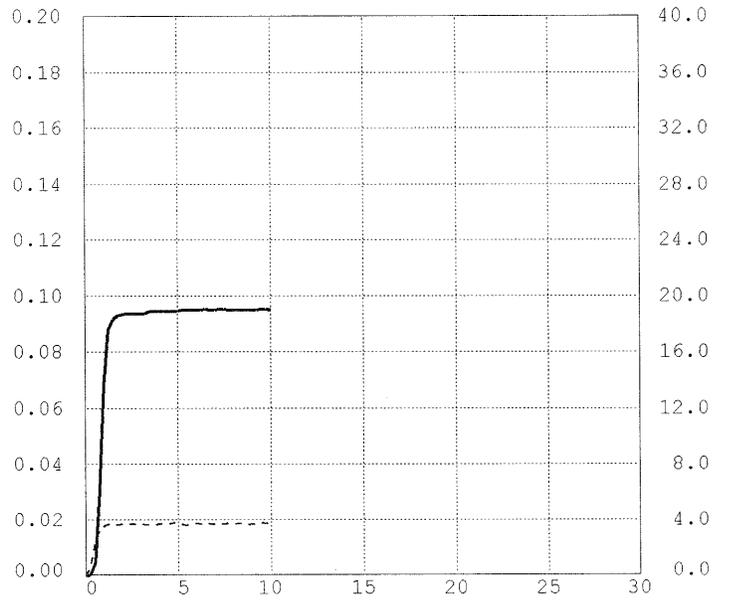

Handwritten signature and notes:
 #248 11/23/11 0837