

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106206

Date: 02/15/2012

Operator Name: RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 11240

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:22
INTERNAL STANDARD	VERIFIED	02:22
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:23
BLANK TEST	0.00	02:23
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:24
BLANK TEST	0.00	02:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	02:25
BLANK TEST	0.00	02:26

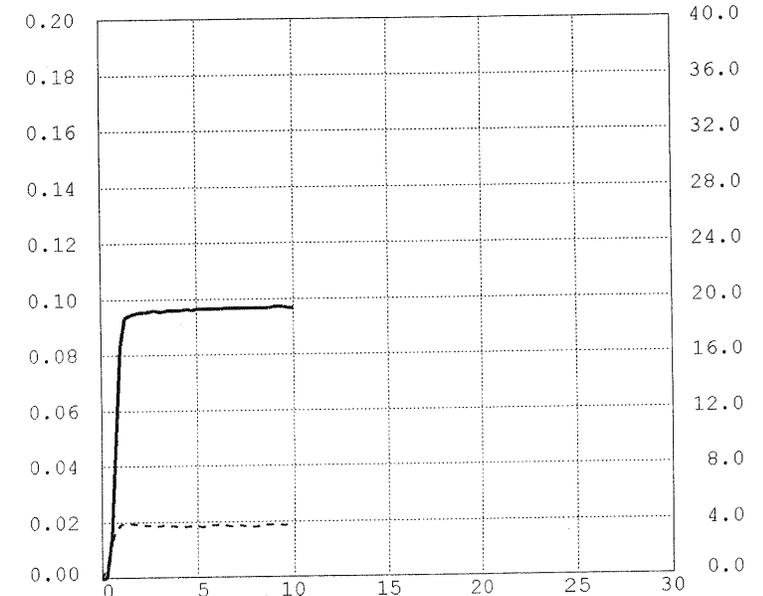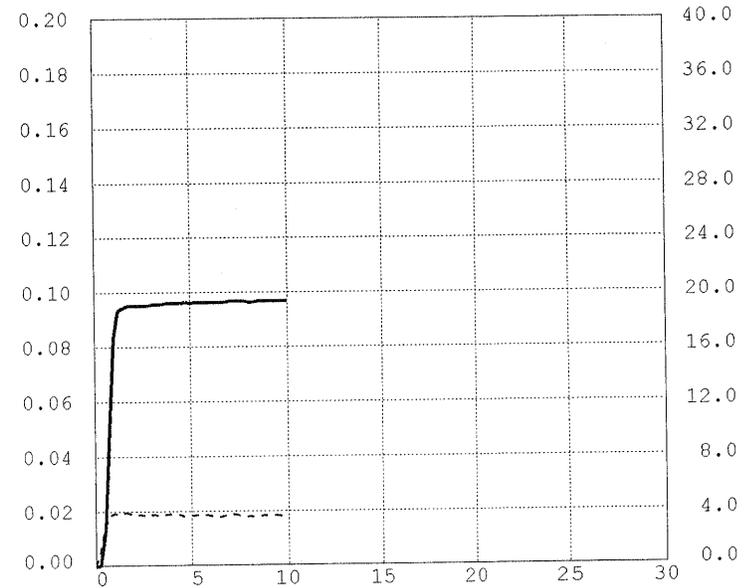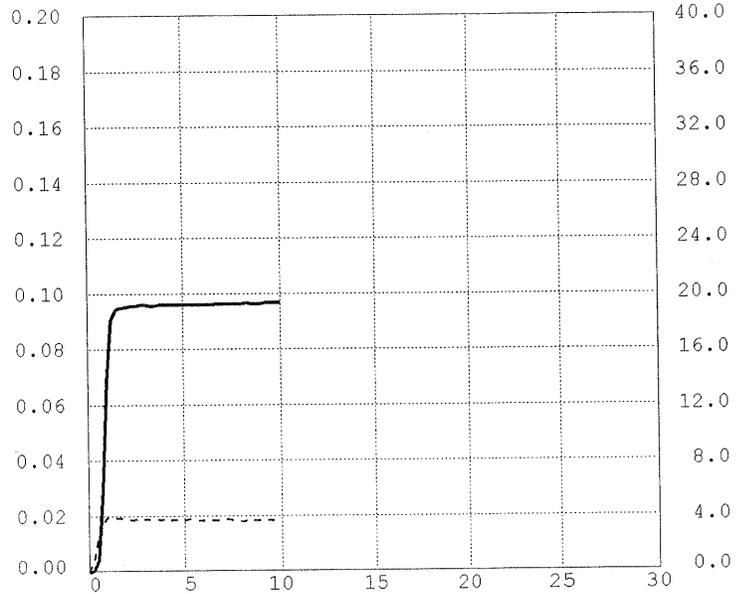

*R. J. Bartlett* #117 02-15-12