

SUPERVISOR TEST




 WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 106206

Date: 03/14/2012

Operator Name: RALPH J BARTLETT
 Permit #: 26222
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 11240

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:35
INTERNAL STANDARD	VERIFIED	03:35
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	03:35
BLANK TEST	0.00	03:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:36
BLANK TEST	0.00	03:37
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	03:37
BLANK TEST	0.00	03:38

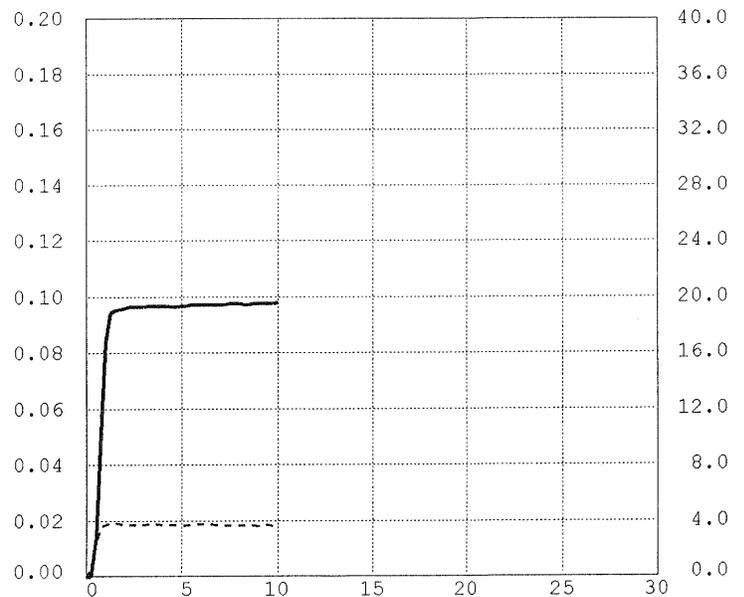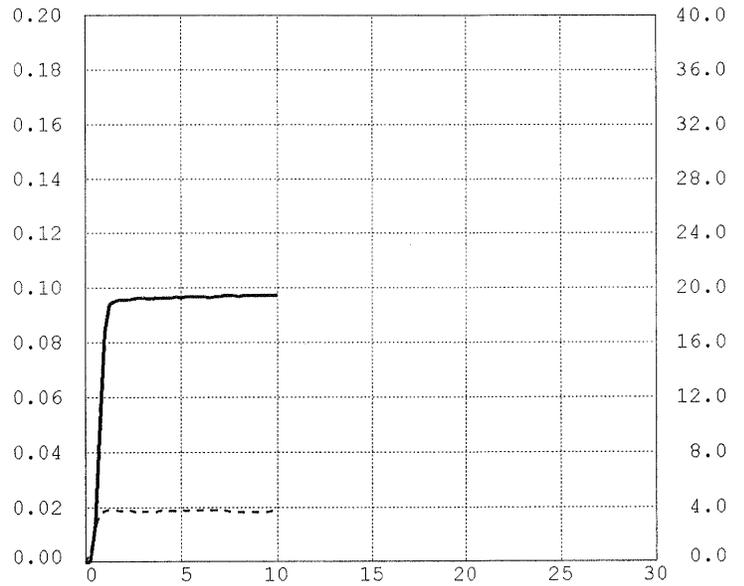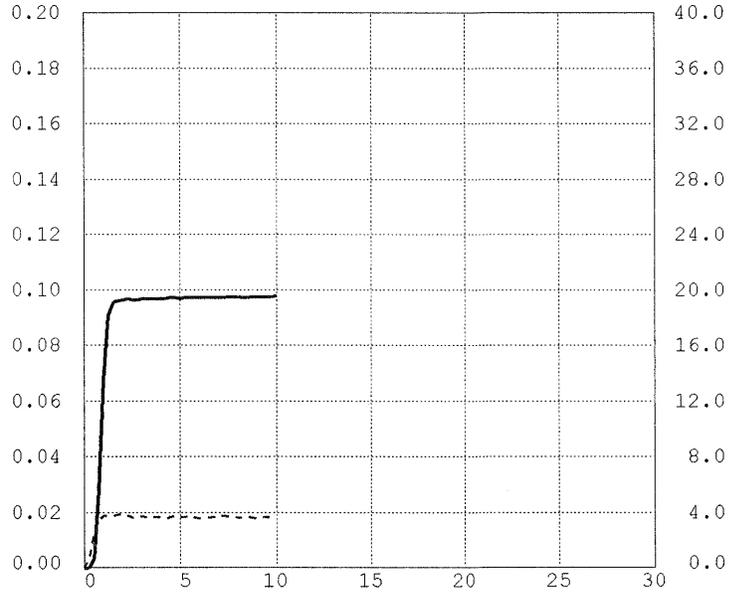

0 IR TO WCO SHELD #162 03-14-12