

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106206

Date: 11/21/2012

Operator Name: CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 12110

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:28
INTERNAL STANDARD	VERIFIED	10:28
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:29
BLANK TEST	0.00	10:29
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	10:30
BLANK TEST	0.00	10:30
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	10:31
BLANK TEST	0.00	10:31

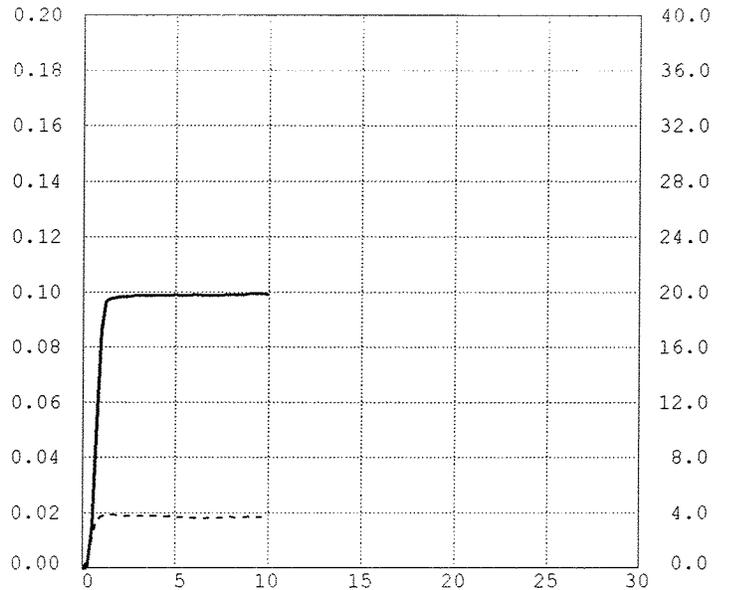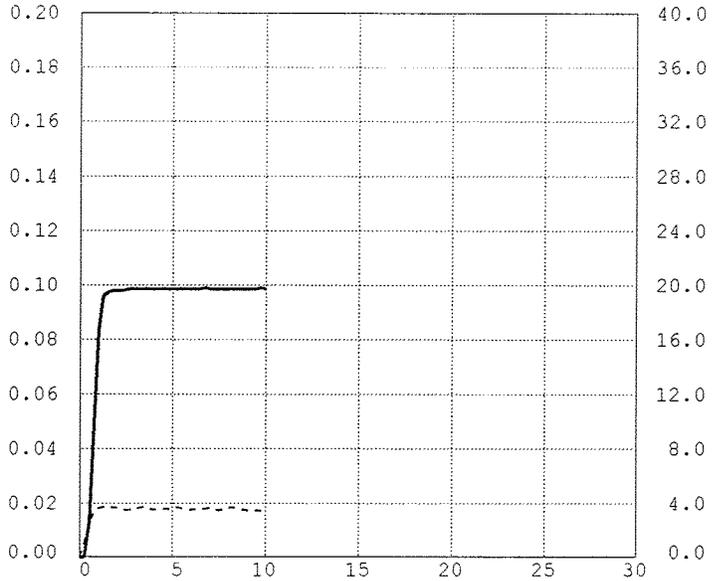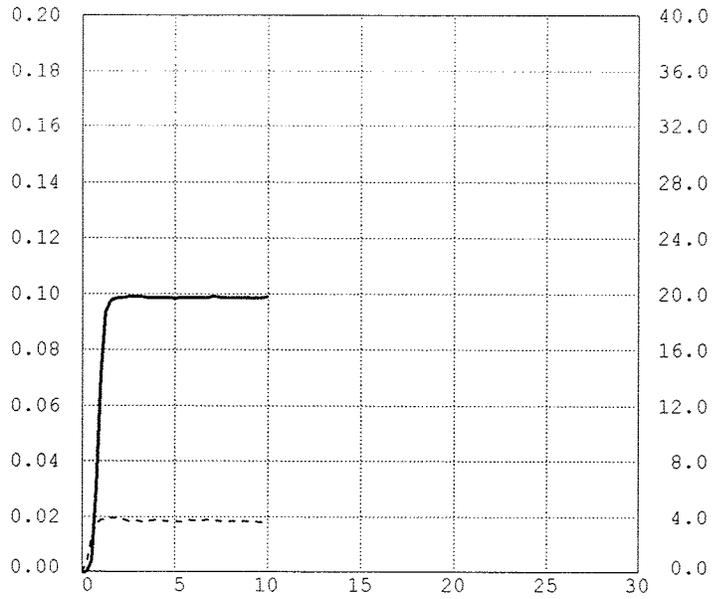

*Charles B. Geisler* #295