

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106206

Date: 12/06/2012

Operator Name: CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 12190

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:58
INTERNAL STANDARD	VERIFIED	07:58
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	07:58
BLANK TEST	0.00	07:59
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	07:59
BLANK TEST	0.00	08:00
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	08:00
BLANK TEST	0.00	08:01

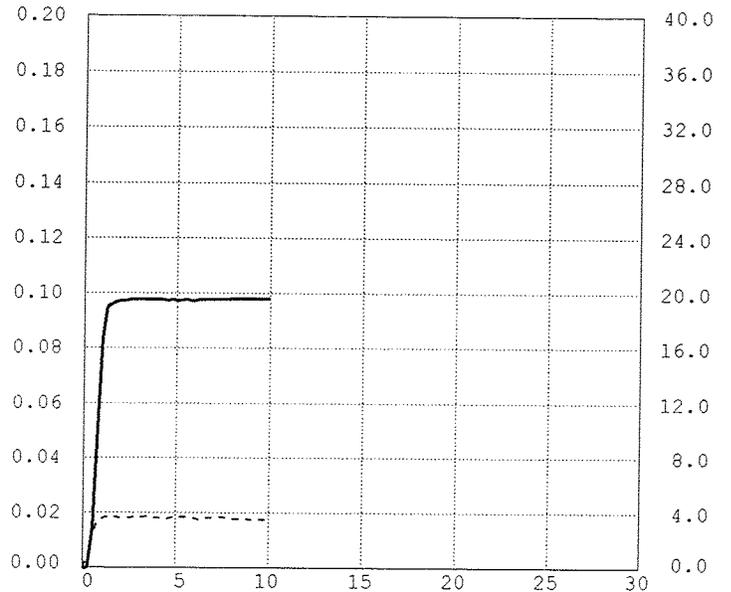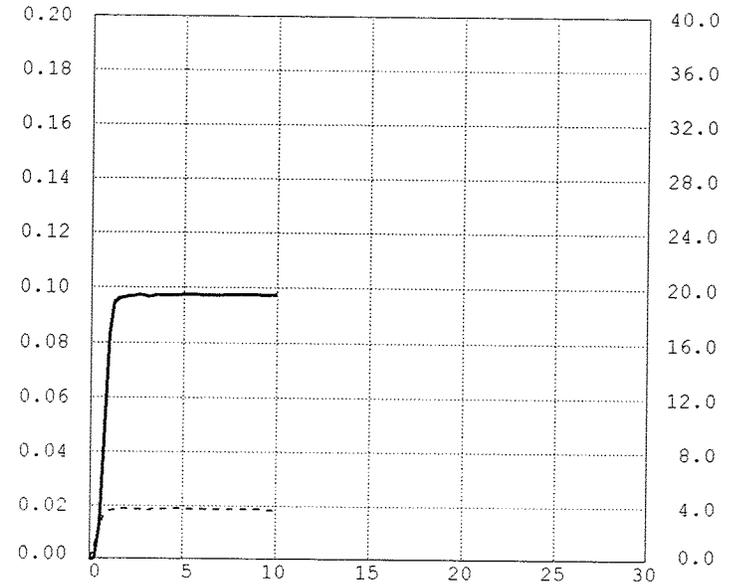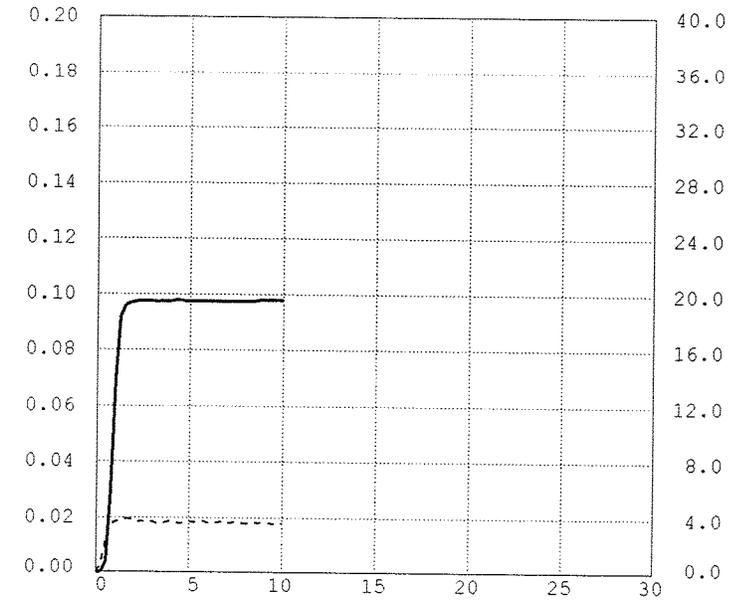

*Charles B. Geisler* #248