

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106206

Date: 08/19/2013

Operator Name: CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 13140

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:19
INTERNAL STANDARD	VERIFIED	18:19
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	18:20
BLANK TEST	0.00	18:20
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	18:21
BLANK TEST	0.00	18:22
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:22
BLANK TEST	0.00	18:23

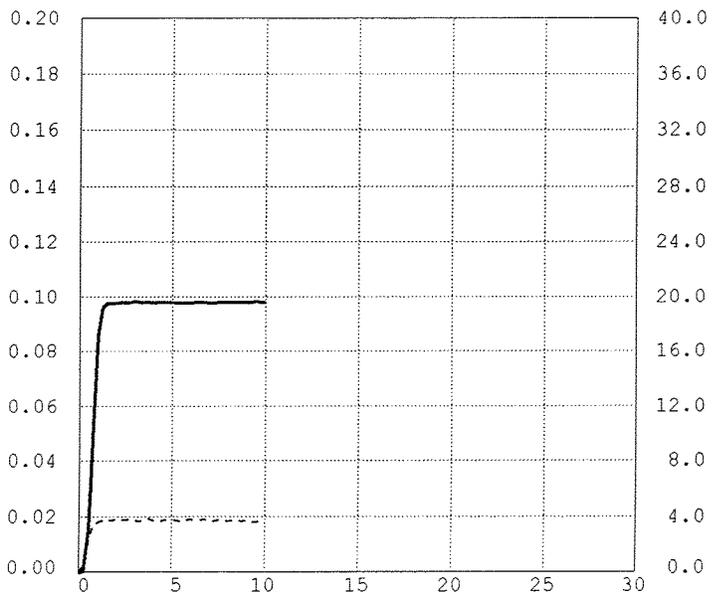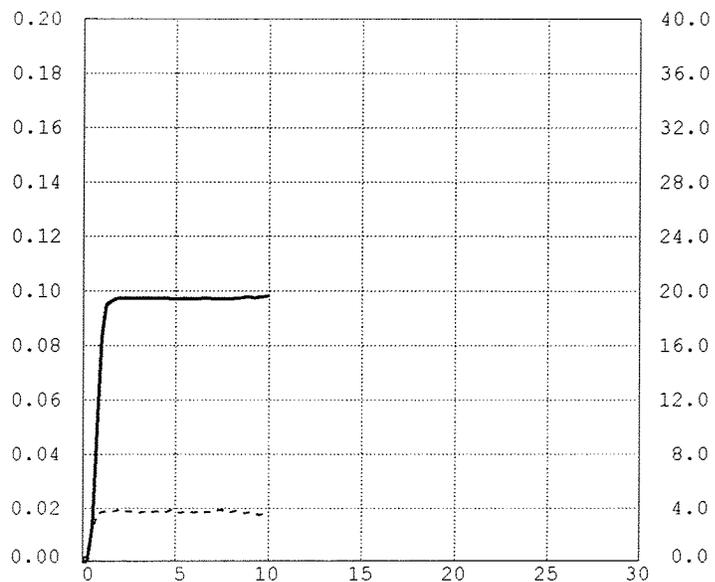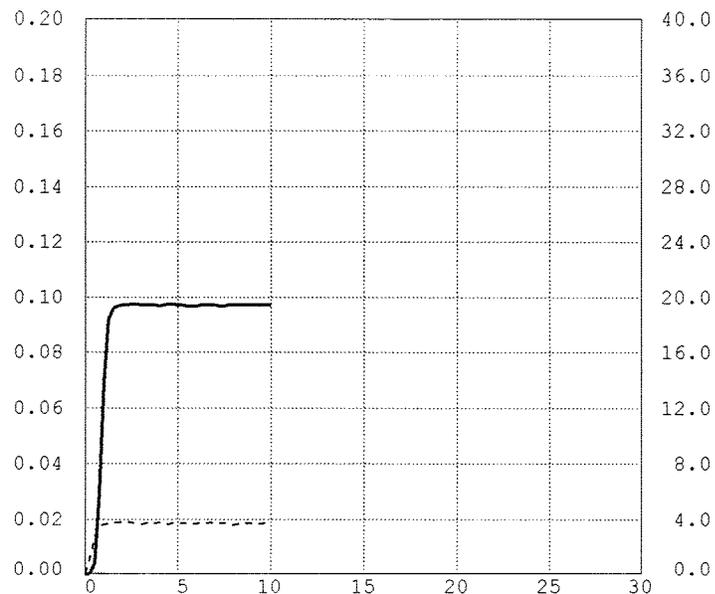

Charles B Geisler #244