

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106206

Date: 11/12/2013

Operator Name: CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 13200

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:40
INTERNAL STANDARD	VERIFIED	08:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:40
BLANK TEST	0.00	08:41
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	08:41
BLANK TEST	0.00	08:42
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	08:42
BLANK TEST	0.00	08:43

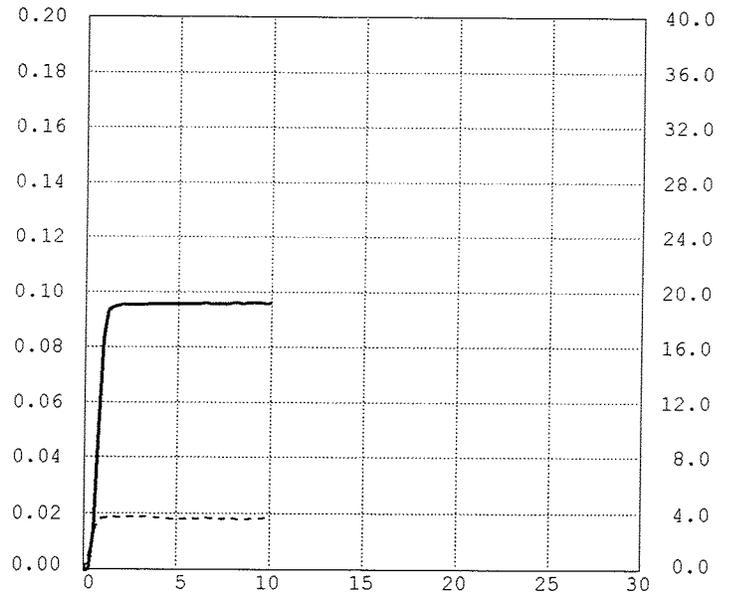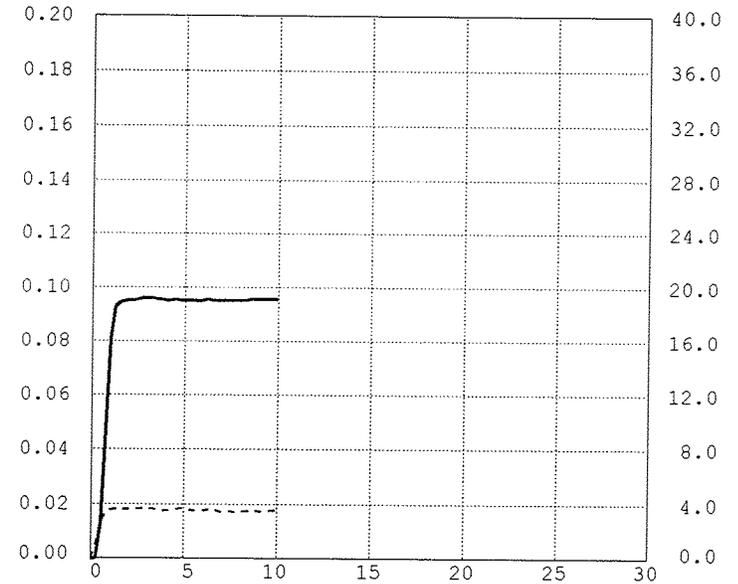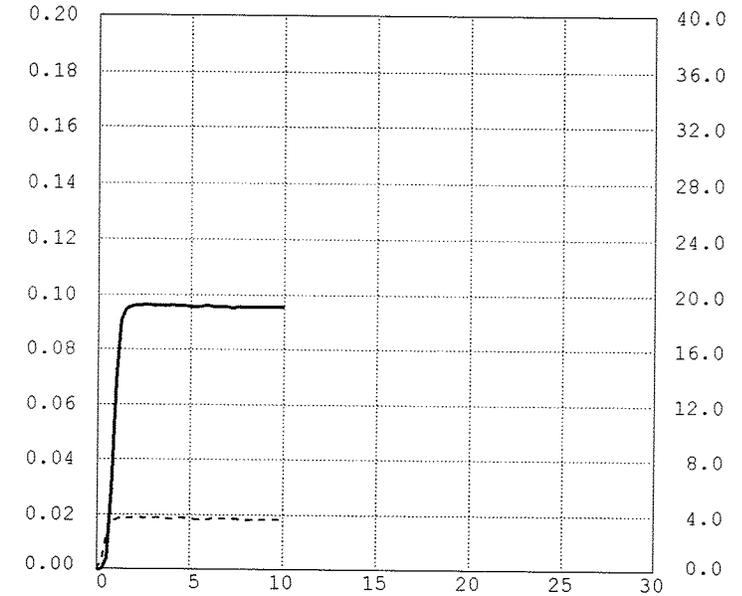

Charles B. Geisler
11/12/13 0843