

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106206

Date: 11/17/2013

Operator Name: CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 13200

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:17
INTERNAL STANDARD	VERIFIED	09:17
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	09:17
BLANK TEST	0.00	09:18
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	09:19
BLANK TEST	0.00	09:19
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	09:20
BLANK TEST	0.00	09:20

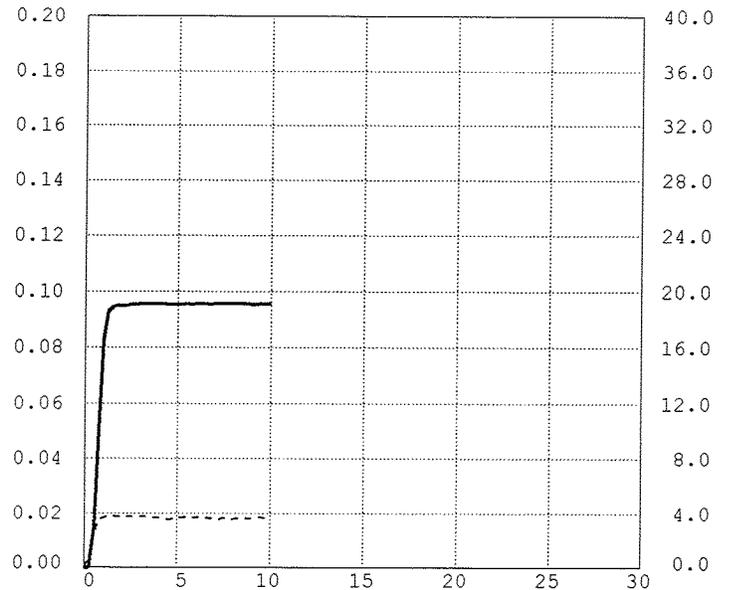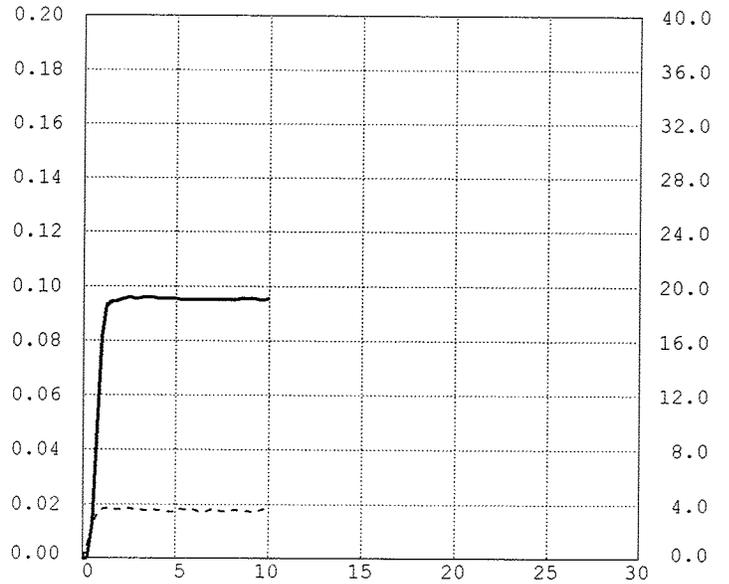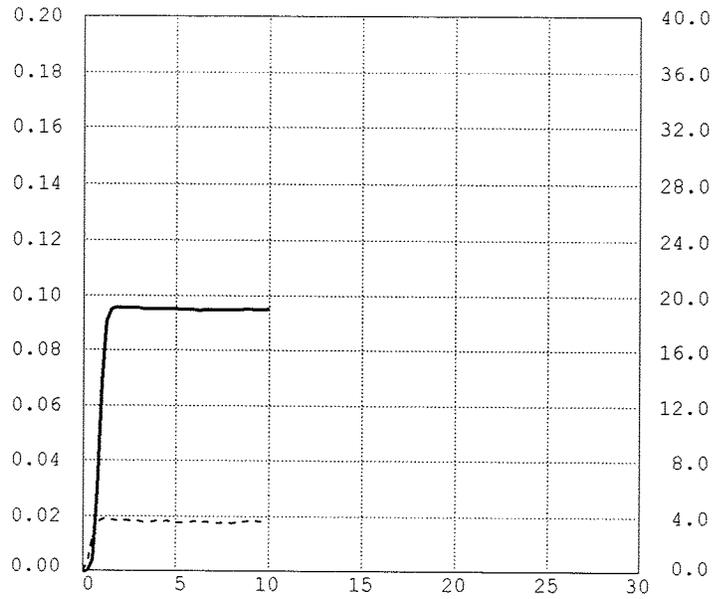

*Charles B. Geisler*  
#248 11/17/13 0922